

**Autonomous Microbial Sampler (AMS), a device for the uncontaminated collection of multiple microbial samples from submarine hydrothermal vents and other aquatic environments.**

Craig D. Taylor<sup>1\*</sup>, Kenneth W. Doherty<sup>2</sup>, Stephen J. Molyneaux<sup>1</sup>, Archie T. Morrison III<sup>3</sup>, John D. Billings<sup>4</sup>, Ivory B. Engstrom<sup>2</sup>, Don W. Pfitsch<sup>2</sup> and Susumu Honjo<sup>2</sup>.

Department of Biology, Woods Hole Oceanographic Institution, MS #33, Woods Hole, MA 02543<sup>1</sup>; McLane Research Laboratories, Inc., Falmouth Technology Park, 121 E. St. Jean Dr., E. Falmouth, MA 02536<sup>2</sup>; Nobska Development Corp., 6 Quissett Circle, Falmouth, MA 02540<sup>3</sup>; Excel Switching, 75 Perseverance Way, Hyannis, MA 02601<sup>4</sup>.

**Running head:** Uncontaminated microbial sampling

\* Corresponding author.

Mailing Address:

Biology Department, Woods Hole Oceanographic Institution, MS #52, Woods Hole, MA 02543.  
Telephone: 508-289-2354  
Fax: 508-457-2076  
E-mail: [ctaylor@whoi.edu](mailto:ctaylor@whoi.edu)

## **Abstract.**

An Autonomous Microbial Sampler (AMS) is described that will obtain uncontaminated and exogenous DNA-free microbial samples from most marine, fresh water and hydrothermal ecosystems. Sampling with the AMS may be conducted using manned submersibles, Remotely Operated Vehicles (ROVs), Autonomous Underwater Vehicles (AUVs), or when tethered to a hydrowire during hydrocast operations on research vessels. The modular device consists of a titanium nozzle for sampling in potentially hot environments (>350°C) and fluid-handling components for the collection of six independent filtered or unfiltered samples. An onboard microcomputer permits sampling to be controlled by the investigator, by external devices (e.g., AUV computer), or by internal programming. Temperature, volume pumped and other parameters are recorded during sampling. Complete protection of samples from microbial contamination was observed in tests simulating deployment of the AMS in coastal seawater, where the sampling nozzle was exposed to seawater containing  $1 \times 10^6$  cells  $\text{ml}^{-1}$  of a red pigmented tracer organism, *Serratia marino rubra*. Field testing of the AMS at a hydrothermal vent field was successfully undertaken in 2000. Results of DNA destruction studies have revealed that exposure of samples of the Eukaryote *Euglena* and the bacterium *S. marino rubra* to 0.5 N sulfuric acid at 23°C for 1 hour was sufficient to remove Polymerase Chain Reaction (PCR) amplifiable DNA. Studies assessing the suitability of hydrogen peroxide as a sterilizing and DNA-destroying agent showed that 20 or 30% hydrogen peroxide sterilized samples of *Serratia* in 1 hr and destroyed the DNA of *Serratia*, in 3 hrs, but not 1 or 2 hrs. DNA AWAY™ killed *Serratia* and destroyed the DNA of both *Serratia* and the vent microbe (GB-D) of the genus *Pyrococcus* in 1 hour.

Keywords: microbiology; samplers; DNA; hydrothermal springs; heat exchange; aseptic.

Regional Index: USA, Massachusetts, Woods Hole; Northern hemisphere, Pacific Ocean.

## **1. Introduction.**

The study of the ecology, diversity and function of microbes in environments such as hydrothermal vents requires the marriage of culture-independent, molecular techniques of DNA sequencing and manipulation to determine the important members of the community and culture-dependent approaches to understand their physiology and functioning. In either case it is essential that samples be obtained that are free from cross-contamination by microbes and microbial DNA from locations other than the site of sampling. Because most devices that are used to sample remote aquatic environments must first be transported through heavily contaminating waters (e.g., air water interface near a ship, upper water column, etc.), means must be provided for protection of collected samples from such contamination or from cross contamination between sampling sites. Since both viable microbes and/or DNA from the habitat of interest are analyzed, protection from both types of contamination is essential.

Obtaining contamination-free microbial samples from the marine and other remote environments has long been of interest (historical account in Zobel, 1941; see also Karl and Dore, 2001), beginning with hydrowire deployed samplers (e.g., Zobel, 1941; Niskin, 1962; Lewis et. al., 1963) that implemented sterile evacuated bottles, bellows-like polyethylene bags or rubber bulbs, respectively, to take samples. Proximity of the sample inlets to the hydrowire and initiation of sampling by unsterile components (e.g., smashing glass inlet tube by messenger or cutting inlet tubing with unsterile knife edge) lead to significant contamination issues, however. To attack the contamination issue, Jannasch and Maddux (1967), developed a swing arm-like sampler that oriented into the current and mechanically drew samples into sterile syringes away

from the hydrowire while a sterile dialysis bag was removed from the sterile inlet prior to sampling. Field tests where the outer surfaces were purposely contaminated with a tracer organism, revealed dramatic improvements in the collection of uncontaminated samples (Jannasch and Maddux, 1967). However, the sampler was not widely implemented.

For sampling in deep waters where hydrostatic pressure is a parameter that can affect microbial viability and growth, pressure-retaining samplers have been implemented in a variety of designs for retrieval of samples in the absence of decompression. Examples include single sample versions with (Jannasch et. al., 1973; Jannasch and Wirsen, 1977) and without (Tabor et. al., 1981) sample inlet protection to reduce the potential for contamination. Bianchi et. al., (1999) expanded the Jannasch et. al. concept to allow up to 8 pressurized samples to be taken during a single deployment, though inlet protection is less rigorous (alcohol-sterilized parafilm).

Microbial studies at hydrothermal vents have catalyzed development of an array of vent samplers that can obtain samples from hot environments. Malahoff, et.al., 2002, for example, have developed a sampling system that is able to take vent fluid samples and maintain both *in situ* temperature and pressure of the sample collected. Once aboard ship subsamples can be transferred to multiple incubators without change in either pressure or temperature. Phillips, et. al., 2003, designed a sampler for the capture, temperature monitoring and *in situ* incubation of hot smoker fluids under vent conditions. In development at the Jet Propulsion Laboratory (<http://www.jpl.nasa.gov/>; A.L. Lane, L.C. French) is an Underwater Volcanic Vent Mission probe, an instrumented titanium probe that can be inserted into warm and hot water hydrothermal vents for *in situ* measurements of temperature, imaging and spectrographic analyses within the vent crevices for evidence of microbial growth in these high-pressure liquid environments.

Recent interests in sampling the Antarctic subglacial lake, Lake Vostok, for unique microbes that have been isolated from the surface biosphere for up to tens of millions of years (e.g., Siegert, et. al., 2003) have catalyzed the ongoing development of sampling devices that can aseptically penetrate the ice sheet to sample the subglacial water column and sediments, while maintaining the two biospheres isolated from one another (e.g., Blake and Price, 2002). Technology is also in development (e.g., Cryobot; Subsurface Ice Probe) to search for evidence of extraterrestrial life in the Martian icecaps (e.g., Cardell et. al., 2004; Carsey et. al., 2005) and possible sub-ice oceans on Europa (e.g., Carsey et. al., 2000; French, et. al., 2001).

Most microbial samplers presently in use do not have sufficient inlet protection to guarantee freedom from exogenous contamination. To address this issue we have developed an Autonomous Microbial Sampler (AMS) that obtains six microbial samples that are free from exogenous microorganisms or DNA. A technical description of the AMS and procedures for sterilization and DNA removal are described herein.

## **2. Materials and Methods.**

### ***2.1. Test organisms and growth conditions.***

*Serratia "marinorubra"*, a red pigmented bacterial strain of *S. plymuthica* was isolated from coastal waters. This aerobic mesophile was grown in Marine Broth 2216 (Difco) at 23°C. The Archaeal strain *Pyrococcus* GB-D was isolated from within the outer surface of a black smoker chimney at a Guaymas Basin 2,020 m deep hydrothermal vent site in the Gulf of California. The hyperthermophilic Archaea was grown anaerobically in sulfur containing modified Marine Broth 2216 (Jannasch, et al. 1992) at 95°C. A culture of the protist *Euglena gracilis*, supplied by Dawn Moran, Woods Hole Oceanographic Institution was grown in Hutner's Medium (ATCC Culture Medium 351) at 20°C.

## ***2.2. Measurement of heat transfer in the Insulated Sample Chamber (ISC).***

The ISC was outfitted with a complete array of Sampling Modules (as shown in Figure 1B), the interior filled with water and the assembly allowed to equilibrate to room temperature overnight. The ISC was then immersed in a refrigerated water bath maintained at a constant 4.5° C. The bath contained a high volume pump that rapidly circulated the water around the ISC, simulating the forced convection that would occur as the submersible, ROV or hydrowire transports the AMS up through the water column. Change in the ISC internal temperature would not begin until the AMS was transported above the thermocline where temperatures exceeded ~3°C. The temperature of the water bath and the interior of the ISC were measured using an Omega Engineering temperature unit equipped with a 1/16” (~1.6 mm; time constant ~2 sec) thermocouple probe. The thermocouple probe was inserted through one of the fittings in the ISC top to measure of the internal temperature of the contained water or placed directly in the refrigerated bath to monitor the external temperature. The ISC was inverted several times every ~10 min to completely mix the interior water to simulate the semi-forced convection that would occur at the interior walls of the ISC during the intermittent lurching and rocking of the AMS during transport through the upper water column and at the sea surface.

## ***2.3. Water Sampling Vessel (WSV) testing.***

A dye study was conducted to quantify the dynamics of mixing of sample into the WSV (Figure 1B; see also Figure 4). The inlet tube of a microgear pump was connected either to a vessel containing a deionized water solution of dilute sodium carbonate (pH ~9) or a vessel of the same alkaline solution containing in addition the dye phenol red (absorbance maximum, 557 nm; pH ~9 assured that the dye was completely in the 557 absorbing form). The outlet tube from the pump was in turn connected to the inlet of a 50 ml WSV. The outlet of the WSV was

connected via narrow bore tubing to a spectrophotometer flow cell contained within a Shimadzu UV-1201 spectrophotometer equipped to record and display the time course of the absorbance at 557 nm of the fluid passing through the flow cell. The dead spaces in the pump and interconnecting tubing were flushed prior to experiments to assure that only the flushing dynamics of the WSV were being measured. Three minute trials were begun by simultaneously starting the pump and the spectrophotometer time course program. Absorbance at 557 nm and the cumulative volume of fluid pumped were recorded by the spectrophotometer and microgear pump software, respectively.

#### ***2.4 Test of the sampling nozzle temperature probe.***

The temperature response of the temperature probe was measured by alternately immersing the sampling nozzle 8-10" (20-25 cm) into approximately 20 L fresh water temperature baths of different temperatures. The sampling nozzle was continuously agitated during measurement at a given temperature. The temperatures of the baths, measured by a mercury thermometer, did not change during the measurements.

#### ***2.5 Contamination assessment studies.***

The AMS apparatus was sterilized by repeated exposure of the sampling end of the nozzle, internal conduiting, Distribution Valve rotor/stator and pump heads to 20% hydrogen peroxide for 3 hr., followed by rinsing with sterile DNA-free deionized water (water and container bag autoclaved 1.5 hr. to remove DNA, see Table 3) contained within the cap removal fluid container (Figure 1A). Sterile 50 mm, 0.45  $\mu\text{m}$  Millipore™ cellulose filters housed in sterilized 50 mm in-line filter holders were filled with sterile deionized water and connected into the AMS as shown in Figure 1B (only one filter unit per channel rather than multiple units

shown). Fluids were distributed through the AMS conduiting via the two software controlled pumps using the software in Manual Operate mode (see Section 3.3.2).

The AMS was tested for its ability to obtain uncontaminated microbial samples using the apparatus illustrated in Figure 2. The test apparatus was constructed from two ~60 cm sections of 4" (~10 cm) transparent schedule 40 PVC piping that were united at the center with a standard 4" (~10 cm) PVC union. The union was modified to form a Tracer Injector using eight 16 ga. lengths of stainless steel tubing glued into place with epoxy and affixed with silicone tubing to form a manifold with flexible injection points as shown in the *Top View* inset of Figure 2. Flowing ~20° C seawater (nominal flow rate 4.3 L min<sup>-1</sup>, filtered to nominal 1 μm using a staged large capacity filter) was introduced at the bottom of the apparatus through a flow diffuser made from an approximately ~20 cm deep bed of 1-1.5 cm marbles to guarantee laminar flow up the pipe until it reached an overflow made from another PVC union fixed with a flow outlet. Prior to use the entire apparatus and tubing was sterilized using a 5% bleach solution, which effectively killed the red pigmented *S. marinorubra* tracer organism. The bleach solution was drained and the apparatus flushed for ~20 minutes with the filtered seawater. During testing, a dye solution (phenol red, in deionized water with pH adjusted to ~8 with sodium bicarbonate) and a ~1 x 10<sup>9</sup> cells ml<sup>-1</sup> culture of the tracer organism grown in 80% seawater (to minimize any chance of the tracer settling below the Tracer Injector) containing 0.1% yeast extract and 0.5% peptone was introduced via peristaltic pump (nominal flow rate, ~4.5 ml min<sup>-1</sup>) into the flowing seawater as shown in the "*Top View*" inset of Figure 2. The dye was implemented to provide a visual guarantee that "contaminated" water did not penetrate into the lower "*uncontaminated*" zone (see Figure 2 photo inset). To guarantee that the "*uncontaminated*" zone was indeed free of *S. marinorubra*, samples were obtained during testing through Luer-Lok™ sample ports in the



side PVC tube using sterile 60 ml syringes. Samples (50 ml) were passed through sterile 50 mm, 0.45  $\mu\text{m}$  Millipore™ cellulose filters housed in sterilized 50 mm in-line filter holders for later culture.

The injected tracer/dye was allowed to come to steady state with the flowing seawater, so that a final density of  $\sim 1 \times 10^6$  cells  $\text{ml}^{-1}$  of tracer organism was attained when fully mixed in the top 1/3 of the “contaminated” zone. Because of the laminar flow of seawater in the test apparatus the tracer suspension tended to migrate up the PVC pipe as coherent tendrils of concentrated tracer (see Figure 2 photo insets) until approximately the halfway point in the “contaminated” zone, where gentle turbulence effectively mixed the tracer with the flowing seawater. Just prior to lowering the AMS nozzle into the test apparatus the peristaltic pump was switched off and the tracer organism/dye front was allowed to migrate  $\sim 30$  cm up the pipe (to allow mixing of the tracer organism with the flowing seawater) before the AMS nozzle was slowly ( $\sim 15$  sec) lowered into the test apparatus. This procedure exposed the AMS nozzle to  $\geq 1 \times 10^6$  cells  $\text{ml}^{-1}$  of tracer organism, to simulate an exposure to contaminating coastal waters prior to sampling. Replicate 75 ml samples were taken in the “Tracer organism-free zone” using the AMS. During some tests one of the AMS filters was skipped during sampling to provide a negative control. The protective caps were machined of autoclavable polypropylene plastic, which are less dense than seawater. Upon removal during sampling, the caps floated to the top of the test apparatus and were retrieved. The floating caps prevented the marble bed from being contaminated by tracer organism during the sampling process.

All of the filters were placed onto the surface of Marine Agar 2216 (Difco) (medium containing sea salts, 0.1% yeast extract, 0.5% peptone and 1.5% agar) for growth of colonies. The nominal 1  $\mu\text{m}$  filtered flowing seawater did contain viable microorganisms that would grow

on the above medium ( $\sim 33$  [ $\pm 6$  SD] cells  $\text{ml}^{-1}$ ) but none contained a red pigment that could be confused with *Serratia marinorubra*, which formed bright red colonies when allowed to grow on the filters for  $\geq 2$  days at room temperature.

## **2.6 Chemical procedures for sterilization and DNA removal in samples.**

### **2.6.1 Acid/base hydrolysis.**

Aliquots (50 $\mu\text{l}$ ) of rinsed suspensions containing  $3 \times 10^4$  cells of *Euglena* or  $2 \times 10^8$  cells of *Serratia* were distributed among a number of sterile 1.5 ml microfuge tubes (6 x 35 mm glass tubes for the 200°C treatment). The microfuge tubes were subjected to alkaline treatment (0.5 N NaOH +/- 1.5N NaCl) or acid treatment (0.5 N H<sub>2</sub>SO<sub>4</sub>) at two temperatures ( $\sim 25$  and  $\sim 50^\circ$  C). Additional treatments involved autoclaving for periods up to 1 hour and exposure to 200°C dry heat for select periods ranging from 0 to 24 hours. At the end of a specified treatment, the aliquots subjected to acid/base hydrolysis were neutralized prior to extraction of DNA.

### **2.6.2. Treatment with hydrogen peroxide or DNA AWAY™.**

Aliquots (50 $\mu\text{l}$ ) of rinsed suspensions containing  $3 \times 10^7$  cells of *Serratia* or *Pyrococcus* were added to microfuge tubes, centrifuged for 7 min. at 12,200 xg (10,000 rpm) to pellet the cells and the supernatant discarded. Hydrogen peroxide (50  $\mu\text{l}$  of 10, 20 or 30% solutions) or DNA AWAY™ (Molecular BioProducts) were added as treatments. Following specified times of 1, 2, or 3 hours the contents were evaporated to dryness so that the treatment solutions did not interfere with the DNA extraction procedure. After drying, 150  $\mu\text{l}$  sterile DNA-free TE buffer (10 mM Tris-HCl, 1 mM EDTA) pH 8 was added to each sample (made from deionized water that was autoclaved 1.5 hr.). A control that was not evaporated was run to rule out DNA destruction by evaporation.

## **2.7. Viability studies.**

Aliquots (50µl) of *Serratia* containing  $4 \times 10^7$  cells added to sterile microfuge tubes. In Treatment I, 50µl of 10%, 20% or 30% hydrogen peroxide were added to yield a final concentration of 5%, 10% or 15%. Treatment II removed any effect of the liquid medium. In this treatment cells were first pelleted by centrifugation, the supernatant discarded and 50µl 10%, 20% or 30% hydrogen peroxide or *DNA AWAY™* added to the tubes. A control tube was re-suspended in sterile 3.5% NaCl. Treatment III checked for effects of residues from the treatments on viability of newly added cells. Tubes from Treatment I containing 15% hydrogen peroxide or *DNA AWAY™* were evaporated to dryness. Fresh cells in medium were pelleted in separate tubes by centrifugation, re-suspended in an equal volume of sterile 3.5% NaCl and 50µl added to each tube. An untreated control tube received 50 µl of the sterile 3.5% NaCl resuspended cells. At designated time intervals of 1, 18 and 41 hours, tube contents were resuspended using a Vortex mixer and then 2µl were spotted on the surface of Marine Agar 2216 plates. Plates were examined over 7 days for growth of red colonies of *Serratia*.

### **2.8. Extraction of remaining DNA for PCR assays.**

DNA was extracted into phenol according to the procedure of Maniatis, et. al., (1982). Any intact cells were lysed by the addition of 417 µl TE buffer, pH 8, 30 µl 10% sodium dodecyl sulfate (SDS) and 3 µl Proteinase K (20 mg/ml) followed by incubation at 37°C for one hour. Next, 100 µl of 5N NaCl and 80 µl CTAB/NaCl were added and the mixed suspension incubated at 65°C for 10 min. An equal volume of phenol/chloroform/isoamyl alcohol (25:24:1) was added and thoroughly mixed before centrifuging in a microfuge at 15,900 xg (13,000 rpm) for 5 min. The supernatant was removed and treated again in the same manner. The supernatant was transferred to another sterile microfuge tube. After adding 0.6 volume of ice-cold isopropanol to precipitate any DNA the preparation was stored at -20°C overnight. The DNA was pelleted in a

microfuge at 15,900 xg (13,000 rpm) for 20 min. and the supernatant discarded. Following the addition of 200 µl ice-cold 70% (vol/vol) ethanol, the preparation was centrifuged in a microfuge as above and the supernatant discarded. After drying under a stream of filtered nitrogen, the precipitated DNA was dissolved in 30µl 3x autoclaved DNA-free de-ionized water.

### **2.9. Polymerase chain reaction (PCR) amplification of 16S rDNA.**

DNA extracted as above was used as template in the PCR procedure. The Bacterial primer pairs 8F(5'-AGRGTGGATCCTGGCTCAG-3') and 1492R(5'-CGGCTACCTTGTTACGACTT-3') as well as Archaeal primer pairs 8F(5'-TCCGGTTGATCCTGCC-3') and 1492R(5'-GGCTACCTTGTTACGACTT-3') used for PCR were produced by Operon Technologies, Inc., Alameda, CA. For *Euglena*, modified forward primer A (ATCTGGTTGATYCTGCCAG) and reverse primer B (CACTTGGACGRCMWCCTAGT) were supplied by Michael S. Atkins, Woods Hole Oceanographic Institution (Atkins et al., 2000). The GeneAmp® PCR System 9700, PE Applied Biosystems, Norwalk, CT was used for all samples. PCR reaction mixtures totaling 100 µl contained 10 µl 10x PCR buffer (Teske, et. al., 2002), 8µl deoxyribonucleoside triphosphate (dNTP), 1 µl of each primer, 76.5-78.5 µl PCR water, 0.5 µl Taq polymerase, and 1-3 µl DNA template.

The PCR amplified samples were loaded on 1% (wt/vol) agarose gels. Following electrophoresis, the gels were stained with ethidium bromide and were examined for DNA bands with the ChemiImager™ 4000 Low Light Imaging System, Alpha Innotech Corp., San Leandro, CA.

### **2.10. Materials.**

All chemicals were of reagent or analytical grade. The following crucial items were obtained from the companies indicated: Temperature probe, Omega Engineering, Inc.; polysulfone filter units, Nalge Nunc International Corporation (Nalgene®); fittings, Upchurch, Inc.; Tedlar™ bags containing sterile, DNA-free deionized water for cap removal, McLane Research Labs, East Falmouth MA.

### **3. Results and Discussion.**

#### ***3.1. Description of the AMS.***

There are two major technical directions one can take in the development of devices for obtaining microbial samples from the deep ocean, that of maintaining both the hydrostatic pressure and temperature of the site of sample collection, or allowing the samples to decompress while focusing on temperature control to protect psychrophiles. Studies of Yayanos and colleagues (Yayanos and Dietz, 1983; Yayanos and DeLong, 1987) suggest that the detrimental effects of decompression on viability of psychrophilic barophiles are relatively slow and secondary to the effects of elevated temperature. While abyssal barophiles (from depths between ~3000-6000 m) that are in culture grow poorly when decompressed, their viability is likely to remain intact during typical periods required for sample recovery and recompression to *in situ* pressures (~4 hr.; Yayanos and DeLong, 1987), so long as low temperatures are maintained. Hadal “obligate” barophiles (from depths >6000 m) are significantly more sensitive to decompression. Cultures of the hadal strain MT-41, for example lose approximately 60% of their viability when decompressed for ~4 hr. (Yayanos and Dietz, 1983). Because of the technical difficulties associated with the routine use of high pressure equipment and the reasonable likelihood of obtaining viable microbes to at least abyssal depths, we chose to focus on a design that does not retain hydrostatic pressure during sample retrieval.

The AMS is shown in Figure 1. The dimensions of the cage are 49.5 cm (19.5”) wide by 46cm (18”) deep by 56 cm (22”) high and the instrument weighs 38.6 kg (85 lbs) in air when the Insulating Sample Chamber (ISC) contains no water and 46.7 kg (103 lbs) in air with the ISC full of water, which would be the typical weight when handled on deck. The instrument weighs 16 kg (35 lbs) in freshwater or 15.4 kg (34 lbs) in seawater (ISC full of water). The major components of the AMS include the following: 1) A sterilizable sampling assembly (Figure 1B) composed of the ISC lid into which are mounted 6 Sampling Modules (SM) that each consist of an assembled series of interchangeable filter units and/or containers for the collection of particulate or water samples according to user needs. The sampling assembly and Sampling Modules are removable for the processing of samples and for sterilization. 2) Fluid controlling components (Figure 1A) comprised of a Distribution Valve (DV) and two positive displacement microgear pumps (Cap Removal Pump, Sampling Pump). 3) A sterilizable Sampling Nozzle and associated umbilicus that will permit uncontaminated sampling of the environment by a submersible or AUV manipulator arm or by direct mounting on the vehicle. A temperature probe has been incorporated into the nozzle to permit continuous measurement and recording of temperature at the site of sampling. 4) A Tattletale 8™-based electronic controller/data recorder for controlling sampling events and interfacing with the user.

A functional schematic of one channel of the AMS is shown in Figure 3. Between sampling events the unit is configured as illustrated in panel A, where the Distribution Valve rotor is positioned between ports, sealing the valve. The first sampling event is initiated by advancement of the valve rotor to Cap Removal Port 1 as shown in panel B, followed by activation of the Cap Removal Pump (P1). Sterilized, DNA-free deionized water (autoclaved 1.5 hr) is briefly pumped, as shown by the arrows (fluid path unshaded), through the valve to a

sampling line “T” manifold, to the umbilicus and Sampling Nozzle. Pressure accumulates within an “energizer coil” that suddenly hydraulically expels the Titanium (or polypropylene for sterility testing described below) Cap to expose a sterile titanium sample inlet tube. P1 is turned off and the Distribution Valve advanced to Sampling Port 1 (panel C). Sample collection begins by activating the Sampling Pump (P2) that draws sample (arrows) from the Sampling Nozzle through Sampling Module 1 of the Sampling Unit, the Distribution Valve, pump P2 and ultimately back into the environment (fluid path unshaded). Upon completion of sampling, pump P2 is turned off and the Distribution Valve is advanced to the next sealed position as shown in panel D. The process is repeated for each of the five remaining samples. Sample contained within the Sampling Module is protected from contamination by the long diffusion path in the Sampling Umbilicus and by the sealed valve.

### ***3.2. Electronic Controller.***

The electronics stack is composed of four 2" x 3" printed circuit boards. The first of these is a Tattletale 8™ (TT8™) single board micro-controller manufactured by Onset Computer Corporation. The system’s control program is run on the TT8’s Motorola 68332 microprocessor and operates the system through the peripheral boards, designed and built by McLane Research Laboratories, East Falmouth, MA.

The first of these boards, the AUX/Stepper, is composed of two portions. The AUX portion accepts power from the main battery or an external power source, provides the regulated voltages necessary to run the rest of the system and a port for connection of a 9-volt battery for memory backup, and the precision circuit to which the sampling nozzle temperature probe is connected. Power to the valve and pumps, is switched under software control. The wiring harness is configured to accept main battery and external power sources simultaneously. Current

is automatically drawn from the higher voltage source. The temperature sensor itself, a thin film or wire wound platinum element, is mounted at the end of the sampling umbilicus (Figure 1A, large circled inset). The Stepper portion of this board contains the hardware for translating TT8™ control signals into the commutation signals that drive the stepper motor of the multiport valve. The binary signal from a slotted disk and a proximity switch is used in conjunction with software algorithms to locate the “home port” and to perform precise port alignment and identification during operation.

The remaining two boards in the stack are both 3-phase motor control boards. Each is associated with one of the two system pumps for operation as described above. The pump circuit is based on a high performance Motorola chip set which is controlled by the TT8™. An analog signal is generated and combined in a supervisory chip with the position of the motor shaft to construct 3-phase commutation signals. A triad of Hall sensors mounted in the motor senses the position of the shaft and the commutation signals are applied to the motor through power FETs in the drive chip. A final chip returns shaft speed information derived from the Hall sensor signals to the TT8™ to close the flow rate control loop in software (see below).

### ***3.3. Software.***

#### ***3.3.1. Operator Interface***

The operator controls the microbial sampler through a layered menu structure. From the Main Menu the operator has access to the real-time clock, system diagnostic and test routines, deployment programming and control, and the instrument data file. The user is presented with the Main Menu when the sampler is first powered up and can return to the Main Menu at anytime.



The communications interface is a standard, 3-wire, RS-232 connection passing ASCII characters. The “operator” works through a laptop PC running a terminal emulator (Cross Cut™) that is provided by Onset Computer Corporation. The interface can also be controlled by a supervisory microprocessor such as might be used to coordinate the actions of an AUV.

### ***3.3.2. Main Menu Options***

**Set Time** – Permits the operator to set the real time clock of the Tattletale 8 micro-controller which is used to schedule sampling in some modes of operation during a deployment and provides time stamps for sample information stored in the instrument data file.

**Diagnostics** – Displays the output of the analog to digital channels monitoring main battery voltage and the microbial sampler temperature sensor. The display is repeated at one-second intervals until terminated by the operator. This option is useful during bench testing and when calibrating the temperature sensor.

**Manual Operation** – Allows direct control of the pumps and valve by the operator through selections from the Manual Operation Menu. This option is intended primarily for bench use during system testing and for instrument preparation prior to deployment.

**Sleep** – Places the instrument in a low power mode to extend battery life. The instrument enters this mode automatically if left without operator input or a task list for more than 20 minutes or during deployment when a task list is complete.

**Deploy System** – Several different modes of operation are available to the operator. In addition to the various sampling modes, the operator has full control over the pumping parameters for each event. As noted above, the pump is dynamically controlled to track a desired flow rate and to protect the sample. Data acquisition is automatic throughout a deployment.

**Offload Data** – During each deployment a data file containing the volumes pumped, estimated sample vessel exchange percentage (discussed below), initial and final probe temperatures, start and stop times, ports used, initial and final battery voltages, and diagnostic messages is created. This information is stored both in battery backed up RAM and in non-volatile flash memory for use in sample analysis. The file is recovered from the instrument in ASCII text format using the “capture to file” capability of the Crosscut™ terminal emulator running on the user’s PC. A time history of each pumping event, including flow rates, cumulative volumes pumped, battery voltages, and probe temperatures, is created. Because of space constraints, this information is stored only in RAM. The pumping histories are also recovered as text files using the terminal emulator. The transfer of the data file is controlled through the Offload Menu.

### ***3.4. Laboratory Testing***

#### ***3.4.1. Water sampling vessel.***

The WSV unit (Figure 4A) is designed to collect filtered or unfiltered water samples. Before a deployment, the WSV is pre-filled with sterile, DNA-free deionized water (autoclaved 1.5 hr) to prevent contamination while compensating for the pressure at depth. Collection entails pumping sample water into the chamber where it mixes with the precharge water before exiting. The vessel inlet consists of a low-shear, ducted nozzle (Figure 4B, inset) that directs the fluid into the sample vessel in a spiral motion to effect complete mixing within the vessel as quickly as possible but without damage to cells (Figure 4B-4F).

If mixing is rapid and complete, sample dilution (with the precharge water) should follow a predictable function of the cumulative pumped volume. To test this, quantitative flushing experiments were conducted at 4 flow rates spanning the range used during typical AMS sampling (Figure 5, 25 - 100 ml min<sup>-1</sup>). Dye-containing sample entering the WSV followed the

same mixing dynamics independent of the flow rate (Figure 5A) and agreed quite well with the algorithm:

$$S_V \approx S_E \times [1 - \exp(-k \times (V - D))] \quad \text{Eq. 1}$$

where  $S_V$  is the absorbance of dye exiting the WSV, representing the concentration of sample after volume  $V$  has been pumped through the vessel,  $S_E$  is the absorbance of the undiluted dye, in this case representing the concentration of the sample in the environment,  $k$  is the dilution constant ( $\text{ml}^{-1}$ ) and  $D$  corrects for the fact that  $\sim 4.2$  ml ( $\sim 8\%$  of the WSV volume) of fluid was pumped before there was any appearance of dye. This is because the dye does not instantaneously mix with the precharge water as seen in Figure 4C, D. Best fit values for  $S_E$ ,  $k$  and  $D$  were  $1.23 (\pm 0.04 \text{ SD})$  absorbance units,  $0.0232 (\pm 0.0024 \text{ SD}) \text{ ml}^{-1}$ , and  $4.2 (\pm 0.9 \text{ SD}) \text{ ml}$  respectively. Dynamics of dye removal from the WSV (i.e., charge water removal) was also measured by pumping in alkaline deionized water (to prevent the phenol red from changing color) (Figure 5B) and fit to the equation:

$$S_v \approx S_E \times \exp(-k(V - D)) \quad \text{Eq. 2}$$

The fit produced essentially the same estimates for  $k$  and  $S_E$  (concentrated dye originally present in the WSV, representing the charge water). Convergence onto an estimate for  $D$  was not possible and was assigned the value  $4.2$  ml to allow best fit estimates of the other variables.

While the above equations did not exactly model the mixing dynamics of the WSV, the best fit estimates obtained were adequate for incorporation into the AMS software to provide a conservative estimate of Sample Vessel Exchange Percentage,  $(S_V/S_E) \times 100$ , so the operator will know when the contents of the WSV is representative of the environment sampled.

### ***3.4.2. Thermal transfer of heat into the Insulated Sample Chamber (ISC).***

A high-density polyethylene (HDPE) Insulating Sample Chamber has been incorporated into the design of the AMS to protect cold collected samples from large temperature excursions during retrieval of the apparatus through warmer waters above the thermocline. Recovery of manned submersibles, ROVs or AUVs can take 30-60 minutes in waters approaching 30° C in the tropics. Deep-sea microbes residing at environmental temperatures of 3° C, typically possess growth temperature maxima of 8-10° C and can tolerate temperatures 6 (±3 SD)° C above growth temperature optima (e.g., Hamamoto, 1999; Madigan et. al., 1997). Above this upper limit, however, viability is dramatically reduced. Moderate to tropical waters at 25-30° C are therefore potentially lethal and protection of collected samples from thermal shock is essential.

Given the complex geometry of the internal array of Sampling Modules (SM), accurate quantification of the heat flow properties of the enclosure required that the dynamics of heat flow be determined experimentally under conditions simulating a typical AMS recovery. The temperature of the water contained within the ISC (i.e., sample temperature) follows a second-order linear-lumped-parameter response equation (Kreith and Bohn, 1993; pp 124-126):

$$T(t) = \left[ m_2 \times \frac{(T_o - T_i)}{(m_2 - m_1)} \times \exp(m_1 \times t) \right] - \left[ m_1 \times \frac{(T_o - T_i)}{(m_2 - m_1)} \times \exp(m_2 \times t) \right] + T_i \quad \text{Eq. 3}$$

Where T(t) is the ISC internal temperature at time t, T<sub>0</sub> is the initial internal temperature (at t=0) and T<sub>i</sub> is the temperature of the infinite heat source or sink (temperature bath or upper ocean). A least squares fit of the data with T<sub>0</sub> = 18.5°C and T<sub>i</sub> = 5°C permitted the determination of rate constants m<sub>1</sub> and m<sub>2</sub> (-5.00 hr<sup>-1</sup>, -0.47 hr<sup>-1</sup>, respectively) that were dependent on the thermal properties of the ISC and assembly of SMs only. It took ~0.13 hr before any change in temperature was detected, which reflects the time required for heat to be conducted through the HDPE wall of the ISC (Figure 6A, closed circles). Once m<sub>1</sub> and m<sub>2</sub> were determined for the ISC under the forced convection conditions at the exterior surface of the container and semi-forced

convection at the interior surfaces of the container, it was possible to estimate temperature change for any temperature regime. Given samples collected from the deep ocean ( $T_0 = 3^\circ \text{C}$ ) and exposure of the AMS to a typically warm upper ocean ( $T_i = 25^\circ \text{C}$ ) for 0.5 and 1 hour, the internal temperature [ $T(t)$ ] would increase by  $\sim 3$  and  $\sim 7^\circ \text{C}$ , respectively. An acceptable temperature increase for cold adapted samples from the deep ocean occurs within this window. If additional thermal protection is necessary, one could place an open cell foam jacket over the ISC for an incremental improvement in insulating capacity (e.g., a  $\frac{1}{4}$ " thick and  $\frac{1}{2}$ " thick jacket would slow heat transfer by  $\sim 10\%$  and  $\sim 20\%$ , respectively).

### ***3.4.3. Temperature Sensor.***

To determine the response of the temperature sensor the Sampling Nozzle was alternately placed into ice water, hot and warm water that was vigorously stirred. Results of the study are shown in Figure 6B. The data (symbols) were least squares fit (solid lines) to Equation 3, where  $T(t)$  is the indicated probe temperature at time  $t$ ,  $T_0$  is the initial temperature of the probe at  $t = 0$ ,  $T_i$  the temperature of the bath into which the probe is immersed and  $m_1$  and  $m_2$ , the temperature response constants,  $\text{min}^{-1}$ ). The data were reasonably fit by the theoretical equations, though the ceramic electrical insulator within the probe, the titanium mounting plate and Sample Inlets had some effect on the dynamics of the Temperature Probe and resulted in small deviations from theoretical two-lump thermal responses. The range of temperature response constants from the experiments shown in Figure 6B were  $m_1, -56 (\pm 13 \text{ SD}) \text{ min}^{-1}$ ;  $m_2, -7.0 (\pm 0.5 \text{ SD}) \text{ min}^{-1}$ . The time required, on average, for the temperature sensor to come within 99% of equilibration was 0.72 min (43 sec). Accurate temperature readings of the environment can therefore be made in just under a minute. Adjustments in probe calibration may be made in software.

### ***3.4.4. Thermal Transfer of Heat in the Sampling Nozzle.***

Because the titanium Sampling Nozzle is connected to an umbilicus that is composed of PEEK™ tubing with an upper temperature limit of approximately 200°C, there is potential for damage if the nozzle is inadvertently or intentionally thrust into very hot vent water (~400°C). To avoid this we incorporated a heat exchanger into the design of the nozzle that would be able to lower the temperature of incoming sample fluid from 400 to 200°C. The heat exchanger was constructed of 0.3175” OD x 0.23144” ID Grade 2 titanium tube with a length that was calculated to mediate the desired change in temperature. The fluid heat loss ( $Q_f$ , Watts) required to lower the temperature of the sample fluid from  $T_{in}$  to  $T_{out}$  (°K) can be found from steam tables (Meyer et. al., 1968) and the following equation:

$$Q_f = m(H_{in} - H_{out}) \quad \text{Eq. 4}$$

where  $m$  is the maximum mass flow of sample fluid through the heat exchange tubing (~60 ml  $\text{min}^{-1} = 1.04 \text{ g sec}^{-1}$ , flow rate at the sampling pump), and  $(H_{in} - H_{out})$  ( $\text{Jg}^{-1}$ ) is the enthalpy change in the incoming and exiting fluid at  $T_{in}$  and  $T_{out}$ , respectively. A linearized estimate for the needed length of the titanium heat exchanger tube was made by equating the heat loss required ( $Q_f$ ) to the heat transferred through the tubing at the mean fluid temperature ( $Q_{ex}$ ):

$$Q_f = m(H_{in} - H_{out}) = Q_{ex} = \frac{\left( \left( \frac{T_{in} + T_{out}}{2} \right) - T_{\infty} \right) L}{\frac{1}{h_{ci} 2\pi r_i} + \frac{\ln(ro/ri)}{2\pi K_{ti}} + \frac{1}{h_{co} 2\pi r_o}} \quad \text{Eq. 5}$$

The titanium heat exchange tubing possessed an inside radius ( $r_i$ ) and outside radius ( $r_o$ ) of 0.116 and 0.159 cm, respectively. The thermal conductivity of Grade 2 titanium,  $K_{ti}$  was determined from tables to be  $0.2 \text{ W cm}^{-2} \text{ °K}^{-1}$  at the temperature range of interest (Kreith and Bohn, 1993). The average heat transfer coefficient between the internal wall of the heat exchange tubing with the internal fluid is  $h_{ci}$  ( $\text{W cm}^{-2} \text{ °K}^{-1}$ ), and the average heat transfer coefficient of the external

wall of the heat exchanger tubing that is in free convection with seawater is  $h_{co}$  ( $W\ cm^{-2}\ ^\circ K^{-1}$ ). Their values are calculated from the equations for forced convection inside the tubing and for a single horizontal cylinder in free convection outside the tubing (Kreith and Bohn, 1993), respectively. These equations were evaluated using the tables of thermodynamic properties of water (Meyer, et. al., 1968) at the average bulk temperature of the fluid  $((T_{in} + T_{out})/2 - T_\infty)$ , where  $(T_{in} + T_{out})/2$  is the average fluid temperature and  $T_\infty$  is the temperature of the surrounding seawater ( $3^\circ C$ ). The term  $1/h_{ci}2\pi r_i$  is the thermal resistance to convection heat transfer per unit length from the sample fluid to the inside wall of the exchange tubing (forced convection,  $cm^\circ KW^{-1}$ ),  $\ln(r_o/r_i)/2\pi K_{Ti}$  is the thermal resistance to conduction of heat per unit length through the titanium wall of the heat exchanger tubing ( $cm^\circ KW^{-1}$ ) and  $1/h_{co}2\pi r_o$  is the thermal resistance to heat transfer from the outer wall of the heat exchange tubing to the surrounding seawater (free convection,  $cm^\circ KW^{-1}$ ). If a value for  $Q_f$  is equated to  $Q_{ex}$  and substituted into Equation 5, the required length of heat exchange can be found by solving for  $L$  (cm).

Because the properties of the sample fluid passing through the heat exchanger dramatically change as it is cooled from a super critical fluid at  $400^\circ C$  to water at  $200^\circ C$  (e.g., velocity decreases  $\sim 3.7x$ , density increases  $\sim 3.7x$ , thermal conductivity increases  $\sim 3.4x$ , specific isobaric heat capacity decreases  $\sim 5.7x$ , viscosity increases  $\sim 3.8x$ ), the calculation in Equation 5 was conducted over smaller increments of the tubing. Rather than conduct a calculation for  $L$  over the whole  $400 - 200^\circ C$  temperature range ( $L_{400-200^\circ C}$ ), where there are large non-linear changes in the parameters of Equations 4 and 5, we chose to calculate and sum the length of heat exchange tubing required to cool the fluid over this range in  $50^\circ C$  steps (i.e.,  $L_{400-200^\circ C} = L_{400-350^\circ C} + L_{350-300^\circ C} \dots + L_{250-200^\circ C}$ ). The parameters in Equations 4 and 5, averaged over the narrower temperature intervals are more easily determined and the summed result,  $L_{400-200^\circ C}$ , more

accurate. At a constant pressure of 275 bar (depth ~2710 m) the value for  $L_{400-200^{\circ}\text{C}}$  was found to be 29 cm (calculation results summarized in Table 1). Because of the errors inherent in determining  $h_{ci}$  and  $h_{co}$ , we added ~20% to the calculated value of  $L_{400-200^{\circ}\text{C}}$  to provide a margin of safety. The length of the heat exchange tubing in the sampling nozzle was therefore increased to 36 cm.

### **3.5 Field testing**

#### ***3.5.1. Assessment of potential for microbial contamination.***

The ability of the AMS sampling nozzle (Figure 1A, inset) to protect collected samples from external contamination was tested using the apparatus illustrated in Figure 2 and procedures described in Methods. The tracer organism, *S. marinorubra* (cell dimensions 0.8-1.0 x 1.0-2.0  $\mu\text{m}$ ), was introduced into filtered seawater flowing in the apparatus at  $4.3 \text{ L min}^{-1}$  at a steady state concentration of  $1.01 (\pm 0.21 \text{ SD}) \times 10^6$  viable cells per ml (determined from samples collected from the “tracer organism-containing zone”). *S. marinorubra* was used as a surrogate for all bacteria when it comes to potential for contamination and has the desired properties that 1) it can be easily seen when grown into colonies (red pigment) and 2) it remains completely viable when introduced and sampled in the test apparatus. Viability of the culture was ~100% when above the viable counts were compared to direct cell counts,  $[1.0 (\pm 0.2 \text{ SD}) \times 10^6$  total cells per ml]. To simulate exposure of the sampling nozzle to contaminating waters prior to sample collection it was slowly lowered through the upper “tracer organism-containing zone” of the test apparatus into the “tracer organism-free zone” as shown in Figure 2 and outlined in Methods. Results of the sampling test are shown in Figure 7 where six 75 ml samples were taken in the “tracer organism-free zone” (i.e., Clean Zone in Figure 7) after the nozzle was purposely contaminated as described above. The filtered source water contained no organisms that grew



into red pigmented colonies, but did contain a host of organisms developing colorless to yellowish colonies ( $\sim 33 [\pm 6 \text{ SD}]$  culturable cells  $\text{ml}^{-1}$ ) and occasional brown colonies (magnified insets). Also, no red colonies were found in control samples collected from the “tracer organism-free zone” just prior to AMS sampling, indicating that the test apparatus was successful in segregating and maintaining a “Clean Zone” separate from the “Contaminated Zone.” Confluent red growth was observed in samples withdrawn from the “Contaminated Zone” as expected. An example of what a “contaminated” AMS sample would look like is shown in the plate labeled “Contam. Example,” which occurred when the contaminated AMS nozzle was accidentally plunged into the marble bed during one test, effectively contaminating the “Clean Zone” with *S. marinorubra*. In a separate experiment (data not shown) the AMS nozzle was lowered past the Tracer Injector (Figure 2) while the peristaltic pump was left running, effectively exposing the nozzle to tendrils (Figure 2, inset; due to the laminar flow regime) of essentially undiluted culture containing  $\sim 10^9$  cells  $\text{ml}^{-1}$  of the tracer organism (vs. the above experiment where the pump was turned off to avoid such high level, less controlled levels of contamination, see Methods). In this experiment 3 AMS samples were obtained in the “Clean Zone” (one sample was skipped as a negative control, which contained no colonies, and two samples were obtained in the “Contaminated Zone” as a positive controls, which resulted in confluent red growth). Two of the 3 AMS samples were free of the tracer organism; one, however, contained a single *S. marinorubra* colony. Only at extreme levels of contamination, approaching 1000x the levels one would typically expect to experience in coastal seawater (e.g., DeLong, et. al., 1999), and  $\sim 2,000$ - $20,000$ x the contamination levels one may experience in the open ocean (Whitman, et. al., 1998, claim  $\sim 5 \times 10^5$  prokaryotes  $\text{ml}^{-1}$  for the open ocean above

200 m and  $\sim 5 \times 10^4 \text{ ml}^{-1}$  below 200 m), is the AMS sampling nozzle less than 100% successful at protecting collected samples from contamination.

### ***3.5.2. Sampling of hydrothermal vents by the AMS.***

Figures 8A and 8B illustrate AMS sampling of various flange and chimney hydrothermal vents. The AMS sampling nozzle proved to be very robust during sampling. Occasional drifting of Alvin during sampling sometimes resulted in “plowing” of the sample nozzle into the rocky surfaces of vent chimneys and inadvertent immersion of the sampling tip into 400°C water without damage. The Perfluoro-elastomer O-rings used to seal the protective caps are in fact rated for continuous exposures to temperatures of 260°C (intermittent exposure to  $\sim 350^\circ\text{C}$ ) without damage and we have proved this to be the case. The O-rings did not carbonize or “weld” the protective caps to the sample inlet, preventing their removal. They remained pliant and were completely undamaged by exposure to  $\sim 400^\circ\text{C}$  water (the titanium metal in fact was slightly discolored by the high temperatures). The  $\sim 12$ ” titanium tube heat exchangers also worked well for cooling very hot samples to temperatures that did not damage the PEEK™ tubing of the umbilicus. During one dive the sampling nozzle was totally immersed in  $\sim 270^\circ\text{C}$  water (figure not shown; not the intended mode of sampling). These temperatures were high enough to melt the boot material used to interface the umbilicus with the nozzle and the plastic material used to consolidate the PEEK™ tubes of the umbilicus. Nevertheless the PEEK™ tubing in the umbilicus remained intact and a good sample was obtained. We believe that with proper sampling procedures the AMS can be used for sampling high temperature water and survive exposure to temperatures  $>350^\circ\text{C}$ .

### **3.6. Testing of Procedures for Sterilization and DNA Removal.**

Various treatments were tested for effective destruction of DNA. Destruction of DNA was verified by conducting Polymerase Chain Reaction (PCR) DNA amplification studies of treated samples of three test organisms, *Euglena gracilis*, a representative of eucaryotic organisms, *S. marinorubra*, a representative of procaryotic organisms (bacteria) and *Pyrococcus* GB-D, a hyperthermophilic sulfur respiring vent archaeal heterotroph. Our intent was to establish a minimum procedure that assures complete destruction of the DNA of these test organisms.

### ***3.6.1. Acid/Base treatment procedures.***

Aliquots of rinsed suspensions of the test organism(s) were distributed among a number of identical microfuge tubes and subjected to autoclaving for up to an hour, alkaline treatment (0.5 N NaOH; 0.5 N NaOH + 1.5N NaCl), or acid treatment (0.5 N H<sub>2</sub>SO<sub>4</sub>) at two temperatures (~25°C and ~50°C or 200°C dry heat for select periods ranging from 0 to 24 hours). At the end of a specified treatment, the acid- or base-treated samples were neutralized, subjected to a standard sodium dodecyl sulfate (SDS) lysis/protease digestion/phenol extraction procedure, followed by alcohol precipitation of DNA for preservation until analysis. Small aliquots of the DNA were subjected to PCR using a universal primer pair for amplification of 23s RNA gene sequences unique to the Eukaryote *Euglena* and 16s RNA gene sequences unique to Bacteria. Analysis of the PCR product by gel electrophoresis was undertaken and ideally resulted in a single band with an intensity (after staining) that is proportional to the initial concentration of intact sequence between the primer pairs. As the DNA-destroying treatment proceeds in time, the probability of a PCR-disrupting lesion appearing in the sequence between the primer pairs increases, resulting in a decrease in PCR product. With increasing treatment time the intensity of

the PCR product band should decrease exponentially. An appropriate treatment will result in no detectable PCR product.

Results of these studies are shown in Figure 9 and Table 2. Figure 9 shows photographs of the agarose gels used for scoring the presence or absence of a discernable DNA band. If there was the slightest indication of a DNA band, as illustrated by lane 6 of both gels 1 and 2, the result was scored positive. Lanes 2 and 5 (among others) in gel 1; lanes 1 and 2 (among others) in gel 2 are examples of samples that contained no amplifiable DNA and were scored negative, (see also Table 2). Positive and negative controls behaved as expected, indicating that the DNA extraction/PCR amplification procedures were working normally and that reagents did not contain exogenous DNA.

*Euglena* cell suspensions were exposed to the following treatments 1) 0.5N NaOH, 2) 0.5 N NaOH + 1.5N NaCl and 3) 0.5N H<sub>2</sub>SO<sub>4</sub> at 25 and 50°C for incubation periods ranging from 15 min to 24 hours. It is clear from the results in Table 3 that exposure to acid was far superior to any of the alkaline treatments. Exposure to 0.5N H<sub>2</sub>SO<sub>4</sub> for 1 hour at 25°C was sufficient to destroy all traces of DNA and <15 min was required at 50°C. DNA could be destroyed by exposure to NaOH as well, but much longer incubations were required. At 25°C a full 24 hours were required to destroy DNA in 0.5N NaOH. The addition of NaCl reduced the time required by half (12 hrs) and incubation at 50°C resulted in a modest improvement with DNA destruction occurring in 5-8 hours. With respect to recycling the AMS for the next deployment, it is abundantly clear that acid treatment is the only procedure that works quickly enough at room temperature to be practical. A one to two hour treatment with 0.5N H<sub>2</sub>SO<sub>4</sub> falls well within a practical time window for recycling the AMS. Based on the effective time intervals observed when *Euglena* was treated with acid, another similarly prepared aliquot of *Serratia* was treated

with 0.5N H<sub>2</sub>SO<sub>4</sub> for periods of 1, 2 and 3 hours. The DNA extraction and PCR procedures were repeated. The treatment also proved effective in destroying DNA from *Serratia* for all three time periods tested.

It is of interest to note that exposure of samples to dry heat (200°C) for 1 hour and autoclaving for 1 hour also destroys DNA. For materials that tolerate these conditions and are of a size to fit into an autoclave or oven, this will be useful in preparation of solutions and hardware for use with the AMS.

### **3.6.2. Hydrogen peroxide and DNA AWAY™ studies.**

We have explored the possibility of using chemical treatments with strong solutions of hydrogen peroxide for both sterilizing the internal conduits of the AMS and for oxidative destruction of exogenous DNA via iron catalyzed radical reactions resulting in the cleavage of the sugar backbone, derivatization of the purine and pyrimidine bases and other oxidative reactions (e.g., Henle and Linn, 1997). Studies in the literature have shown that 30% hydrogen peroxide was effective for sterilizing glass surfaces and biological indicator disks inoculated with viable cells and spores of *Bacillus subtilis* and *Bacillus stearothermophilus* after < 30 min exposure at room temperature (Wilkins, et.al., 1994). If hydrogen peroxide is effective, the AMS could be sterilized and freed of exogenous DNA without disassembly of the unit. This would greatly simplify the logistics of recycling the AMS between deployments. Effectiveness of hydrogen peroxide and the commercial product DNA AWAY™ for destroying *Serratia* DNA is also shown in Table 3. Hydrogen peroxide at 20% or 30% will destroy DNA after a 3 hr exposure, but not at the shorter exposure times of 1 or 2 hrs. DNA AWAY™ was effective at destroying DNA in the shortest incubation period tested, 1 hr. Tests of the effectiveness of DNA

AWAY™ were made on the additional test organism, *Pyrococcus* GB-D. As shown in Table 3, it was identically effective at destroying the DNA of this organism as it was for *Serratia*.

We have conducted a viability study with our bacterial test organism in which cell suspensions and pelleted cells were exposed to final concentrations of ~5, 10, 15, 20 and 30% hydrogen peroxide for 1 – 24 hours (Table 4). When  $\sim 1.6 \times 10^6$  cells were then plated on a nutrient medium no growth was found in any of the cases, suggesting that hydrogen peroxide can be quite effective at killing vegetative bacterial cells. Residues left over after air drying hydrogen peroxide treated cultures did not appear to affect the viability of freshly added cells.

The commercial product, DNA AWAY™, made by Molecular BioProducts is used for treatment of glass, plastic ware and stainless steel to destroy DNA and may also have application with the AMS. Experiments shown in Table 4 suggest DNA AWAY™ does kill our test bacterium, *S. marinorubra* with the same effectiveness as hydrogen peroxide, though this result is not likely to hold for all organisms. If DNA AWAY™ is used for treating AMS conduits, care should be taken to assure that it is completely removed to avoid killing sample organisms or destroying desired sample DNA. Residues left from treatment after air-drying, however, do not affect viability of *Serratia* or destroy DNA of either test organism.

The experiments conducted indicate that chemical means can be implemented for the combined requirement of sterilization and destruction of DNA. Exposure of the AMS conduits to high strength (20%) hydrogen peroxide for at least 3 hrs will be effective for this dual purpose. It is of interest to note that titanium is chemically attacked by 30% hydrogen peroxide, as evidenced by the appearance of a yellowish color in the hydrogen peroxide solution and probably should be avoided. This was not observed when titanium was exposed to 20% hydrogen peroxide. If desired, additional exposure of the conduits to the commercial agent DNA

AWAY™ will provide an increased margin of safety with respect to the removal of exogenous DNA.

### **Acknowledgments.**

This work was supported by a DOC/NOAA Small Business Innovative Research Award, Contract No. 50-DKNA-9-90116 awarded to McLane Research Laboratories, Inc. and (via subcontract) to the Woods Hole Oceanographic Institution. Some of the microbial testing work was also supported by the National Science Foundation, Grant No. IBN-0131557 and the Woods Hole Oceanographic Inst. Deep Ocean Exploration Institute Grant No. 25051131. We acknowledge and appreciate the excellent technical assistance of Dr. Konstantinos Ar. Kormas for PCR analysis and Dr. Fredrik Thwaites for reviewing the heat conduction studies presented.

## References

- Atkins, M.S., A.P. Teske and R.O. Anderson. 2000. A survey of diversity at four deep-sea hydrothermal vents in the Eastern Pacific Ocean using structural and molecular approaches. *J. Eukaryot. Microbiol.* 47: 400-411.
- Bianchi, A., J. Garcin and O. Tholosan. 1999. A high-pressure serial sampler to measure microbial activity in the deep sea. *Deep-Sea Res. I.* 46: 2129-2142.
- Blake, E.W. and B. Price. 2002. A proposed sterile sampling system for Antarctic subglacial lakes. *Mem. Inst. Polar Res., Spec. Issue.* 56: 253-263.
- DeLong, E.F., L.T. Taylor, T.L. Marsh and C.M. Preston. 1999. Visualization and enumeration of marine planktonic Archaea and Bacteria by using polyribonucleotide probes and fluorescent *in situ* hybridization. *Appl. Environ. Microbiol.* 65: 5554-5563.
- Cardell, G.; Hecht, M. H.; Carsey, F. D.; Engelhardt, H.; Fisher, D.; Terrell, C.; Thompson, J., 2004. The subsurface ice probe (SIPR): A low-power thermal probe for the martian polar layered deposits. 35th Lunar and Planetary Science Conference, March 15-19, 2004, League City, Texas, Abstract No. 2041.
- Carsey, F.D., G-S. Chen, J. Cutts, L. French, R. Kem, A.L. Lane, P. Stolorz, W. Zimmerman and P. Ballou. 2000. Exploring Europa's ocean: A challenge for marine technology of this century. *Mar. Technol. Soc. J.* 33: 5-12.
- Carsey, F.D., L.W. Beegle, R. Nakagawa, J.O. Elliott, J.B. Matthews, M.L. Coleman, M.H. Hecht, A.B. Ivanov, J.W. Head, S. Milkovich, D.A. Paige, A.N. Hock, D.I. Poston, M. Fensin, R.J. Lipinski, and T.M. Schriener. 2005. Palmer Quest: a Feasible Nuclear Fission "Vision Mission" to the Mars PolarCaps. 36th Annual Lunar and Planetary Science Conference, 36: Abst. no.1844.



- French, L.C., F.S. Anderson, F.D. Carsey, J.R. Green, A.L. Lane and W.F. Zimmerman. 2001. Subsurface Exploration Technologies and Strategies for Europa. Forum on Innovative Approaches to Outer Planetary Exploration 2001-2020. 30.
- Hamamoto, T. 1999. Deep-Sea Psychrophiles. In K. Horikoshi and K. Tsujii (Eds.). Extremophiles in Deep-Sea Environments. Springer, Tokyo, Japan. 316 pp.
- Henle, E.S. and S. Linn. 1997. Formation, prevention, and repair of DNA damage by iron/hydrogen peroxide. J. Biol. Chem. 272: 19095-19098.
- Jannasch, H.W., C.O. Wirsen and C.L. Winget. 1973. A bacteriological pressure-retaining deep-sea sampler. Limnol. Oecnaogr. 20: 661-664.
- Jannasch, H.W., Wirsen, C.O., 1977. Retrieval of concentrated and undecompressed microbial populations from the deep sea. Appl. Environ. Microbiol. 33: 642-646.
- Jannasch, H.W., C.O. Wirsen, S.J. Molyneaux and T.A. Langworthy. 1992. Comparative physiological studies on hyperthermophilic Archae isolated from deep-sea hot vents with emphasis on *Pyrococcus* strain GB-D. Appl. Environ. Microbiol. 58: 3472-3481.
- Jannasch, H.W. and W.S. Maddux. 1967. A note on bacteriological sampling in seawater. J. Mar. Res. 25: 185-189.
- Karl, D.M. and J.E. Dore. 2001. Microbial ecology of the sea: Sampling, subsampling and incubation considerations. In: J.H. Paul (Ed.), Methods in Microbiology. 30: 13-39.
- Kreith, F. and M.S. Bohn. The Principles of Heat Transfer. 5<sup>th</sup> Edition. West Publishing Co., St Paul, MN. 720 pp. 1993.
- Lewis, W.M., McNail, O.D. and Summerfelt, R.C., 1963. A device for taking water samples in sterile bottles at various depths. Ecology 44, 171-173.

- Madigan, M.T., J.M. Martinko and J. Parker. 1997. Brock, Biology of Microorganisms. 8<sup>th</sup> Edition. Prentice Hall, Upper Saddle River, NJ. 986 pp.
- Malahoff, A., T. Gregory, A. Bossuyt, S. Donachie and M. Alam. 2002. A seamless system for the collection and cultivation of extremophiles from deep-ocean hydrothermal vents. IEEE Journal of Oceanic Engineering. 27: 862-869.
- Maniatis, T., E.F. Fritsch and J. Sambrook. 1982. Molecular Cloning, A Laboratory Manual. Cold Spring Harbor Laboratory, Cold Spring Harbor, NY.
- Meyer, C.A., R.B. McClintock, G.J. Silvestri and R.C. Spencer, Jr.. 1968. 1967 ASME Steam Tables, Second Edition. The Society of Mechanical Engineers, New York, N.Y. 328 pp.
- Niskin, S.J. 1962. A water sampler for microbiological studies. Deep-Sea Res. 9: 501-503.
- Phillips, H., L.E. Wells, R.V. Johnson II, S. Elliott and J.W. Deming. 2003. LAREDO: a new instrument for sampling and *in situ* incubation of deep-sea hydrothermal vent fluids. Deep-Sea Res. I. 50: 1375-1387.
- Siegert, M.J., M. Tranter, J.C. Ellis-Evans, J.C. Priscu and W.B. Lyons. 2003. The hydrochemistry of Lake Vostok and the potential for life in Antarctic subglacial lakes. Hydrol. Process. 17: 795-814.
- Tabor, P.S., J.W. Deming, K. Ohwada, H. Davis, M. Waxman, R.R. Colwell. 1981. A pressure-retaining deep ocean sampler and transfer system for measurement of microbial activity in the deep sea. Microb. Ecol. 7: 51-65.
- Teske, A., K-U. Hinrichs, V. Edgcomb, A. Vera-Gomez, D. Kysela, S.P. Sylva, M.L. Sogin and H.W. Jannasch. 2002. Microbial diversity of hydrothermal sediments in the Guaymas Basin: evidence for anaerobic methanotrophic communities. Appl. Environ. Microbiol. 68: 1994-2007.

- Whitman, W.B., D.C. Coleman and W.J. Wiebe. 1998. The unseen majority. *Proc. Natl. Acad. Sci. USA* 95:6578-6583.
- Wilkins, D.L, P.Y Chung, P.Y. Tsuchiya, I.F. Wessels and A.J. Zuccarelli. 1994. Microbiologic evaluation of a hydrogen peroxide sterilization system. *Ophthalmic Surg.* 25:690-694.
- Yayanos, A.A. and A.S. Dietz. 1983. Death of a hadal deep-sea bacterium after decompression. *Science.* 220: 497-498.
- Yayanos, A.A. and E.F. DeLong. 1987. Deep-sea bacterial fitness to environmental temperatures and pressures. In: H.W. Jannasch, R.E. Marquis and A.M. Zimmerman (Eds.). *Current Perspectives in High Pressure Biology.* Academic Press, Orlando, Florida. 16-32.
- Zobell, C.E. 1941. Apparatus for collecting water samples from different depths for bacteriological analysis. *J. Mar. Res.* 4: 173-188.

## **Figures.**

**Figure 1.** Autonomous Microbial Sampler (AMS). Panel A, external hardware. Panel B, sample retaining components.

**Figure 2.** Apparatus for testing the ability of the AMS to obtain uncontaminated samples.

**Figure 3.** Functional schematic of one channel of the AMS fluid handling components.

**Figure 4.** AMS Water Sampling Vessel (WSV) and demonstration of effectiveness of mixing using a dye.

**Figure 5.** Mixing dynamics in 50 ml AMS Water Sampling Vessel. Panel A, fraction of sample contained in the WSV vs. volume of sample pumped through system. Panel B, fraction of precharge water remaining in the WSV vs. volume of sample pumped through system.

**Figure 6.** Time course measurements of the thermal properties of AMS components. Panel A, thermal dynamics of the Insulated Sample Chamber. Panel B, response of the sampling nozzle temperature sensor to abrupt temperature changes (symbols, measured data; solid lines, least square fits to equation 3). Best fit parameter values are shown in the insets.

**Figure 7.** Protection of samples from contamination after exposure of the AMS nozzle to a  $1 \times 10^6$  viable cells  $\text{ml}^{-1}$  seawater suspension of *S. marinorubra*.

**Figure 8.** AMS sampling at hydrothermal vents using DSV Alvin. Panel A, sampling at a flange vent (variable temperature between 140-200°C) ambient and at the Lobo site on Endeavor Ridge, Juan de Fuca Ridge vent field ( $\sim 47^\circ 53' \text{N}$ ,  $\sim 129^\circ 9' \text{W}$ ; R/V Atlantis cruise AT03-54). Panel B, sampling of high temperature vent fluid ( $\sim 280^\circ \text{C}$ ) emanating from the Chowder Hill vent site at Juan de Fuca Ridge, ( $48^\circ 27.6' \text{N}$ ,  $\sim 128^\circ 42.6' \text{W}$ ).

**Figure 9.** Examples of agarose gels of PCR amplified *Euglena gracilis* DNA after indicated treatments.

1 **Tables.**

2

3 **Table 1. Average heat transfer coefficients<sup>1</sup> ( $\bar{h}_{ci}$ ,  $\bar{h}_{co}$ , and  $K_{Ti}$ ), average heat**  
 4 **loss ( $Q_f$ ) and computed length ( $L$ ) of titanium heat exchange tubing required**  
 5 **to reduce the temperature of water by the indicated 50°C increments ( $\Delta T_f$ ).**  
 6

$\Delta T_f$ (°C)	$Q_f$ (Watt)	$\bar{h}_{ci}$ (Wcm <sup>-2</sup> °K <sup>-1</sup> )	$\bar{h}_{co}$ (Wcm <sup>-2</sup> °K <sup>-1</sup> )	$K_{Ti}$ (Wcm <sup>-1</sup> °K <sup>-1</sup> )	$\bar{T}-T_\infty$ (°C)	$L$ (cm)
400-350	799	0.690	0.350	0.2	372	11.0
350-300	296	0.620	0.319	0.2	322	5.2
300-250	252	0.590	0.281	0.2	272	5.7
250-200	233	0.552	0.242	0.2	222	7.2
400-200					<b>Sum</b>	<b>29.1</b>

7

8 <sup>1</sup>Pressure of system, 275 bar. See Equations 4 and 5 and the associated text for definition and  
 9 units of indicated parameters.

10

11  $\Delta T_f$ = the 50°C temperature interval over which the average heat transfer properties were  
 12 determined.

13

14  $T_\infty$  = temperature of the infinite sink,  $\bar{T} = \frac{T_{in}+T_{out}}{2}$  is the average fluid bulk temperature over the  
 15 indicated 50° temperature interval. See Equation 5.

16 **Table 2. Score of presence (+) or absence (-) of *Euglena gracilis* DNA in the**  
 17 **gels of Figure 8 after treatments.**

18

<b>Gel 1</b>				
<b>Well Number</b>	<b>Incubation Temperature (°C)</b>	<b>Hr. Incubated</b>	<b>Treatment</b>	<b>Score</b>
1	50	0.25	NaOH	+
2	Negative Control	0	NaOH + NaCl	-
3		0.25	NaOH + NaCl	+
4	25	0.25	H <sub>2</sub> SO <sub>4</sub>	+
5	50	0.25	H <sub>2</sub> SO <sub>4</sub>	-
6	200	0.25	Dry	+
7	25	18	NaOH	+
8	50	24	NaOH	-
9	25	18	NaOH + NaCl	-
10	50	24	NaOH + NaCl	-
11	Negative Control	0	Reagent	-
12	Positive Control	0	Untreated cells	+
13	---	---	NA	-
14	---	---	NA	-
15	---	---	DNA Marker	+
<b>Gel 2</b>				
1	50	2	H <sub>2</sub> SO <sub>4</sub>	-
2	200	2	Dry	-
3	121	0.5	Autoclave	+
4	25	2	NaOH	+
5	50	5	NaOH	-
6	25	2	NaOH + NaCl	+
7	50	5	NaOH + NaCl	+
8	25	0.5	NaOH	+
9	50	1	NaOH	+
10	25	0.5	NaOH + NaCl	+
11	50	1	NaOH + NaCl	+
12	25	1	H <sub>2</sub> SO <sub>4</sub>	-
13	50	1	H <sub>2</sub> SO <sub>4</sub>	-
14	200	1	Dry	-
15	121	0.25	Autoclave	+
16	25	24	H <sub>2</sub> SO <sub>4</sub>	-
17	50	24	H <sub>2</sub> SO <sub>4</sub>	-
18	200	24	Dry	-
19	Negative Control	0	NaOH	-
20	---	---	DNA Marker	+

19 NA = lane not applicable to present experiment.

20 (+) indicates visible DNA bands on the gels, (-) indicates no visible bands.

21 (---) = treatment not conducted or relevant.

22 **Table 3. Destruction of *Euglena gracilis*, *S. marinorubra* and *Pyrococcus* GB-**  
 23 **D DNA following intervals of chemical and high temperature treatments.**

24  
25

*Euglena gracilis*

Treatment (hr.)	Pos. Ctrl	Neg. Ctrl	Treatment							
			25°C			50°C			200°C	121°C
			0.5 N NaOH	1.5 N NaCl + 0.5 N NaOH	0.5 N H <sub>2</sub> SO <sub>4</sub>	0.5 N NaOH	1.5 N NaCl + 0.5 N NaOH	0.5 N H <sub>2</sub> SO <sub>4</sub>	Dry Heat	15 psi Autoclave
0 <sup>1</sup>	+	---	---	---	---	---	---	---	---	---
0 (cell free) <sup>2</sup>	---	-	-	-	---	---	---	---	---	---
0.25	---	---	+	+	+	+	+	-	+	+
0.5	---	---	+	+	+	+	+	-	+	+
1	---	---	+	+	-	+	+	-	-	-
2	---	---	+	+	-	+	+	-	-	---
5	---	---	+	+	-	-	+	-	-	---
8	---	---	+	+	-	-	-	-	-	---
12	---	---	+	-	-	-	-	-	-	---
18	---	---	+	-	-	-	-	-	-	---
24	---	---	-	-	-	-	-	-	-	---

26  
27

*Serratia marinorubra*

Treatment (hr.)	Pos. Ctrl <sup>1</sup>	25°C				
		0.5 N H <sub>2</sub> SO <sub>4</sub>	30% H <sub>2</sub> O <sub>2</sub>	20% H <sub>2</sub> O <sub>2</sub>	10% H <sub>2</sub> O <sub>2</sub>	DNA AWAY™
0 <sup>1</sup>	+	---	---	---	---	---
1.3	---	-	---	---	--	---
2.3	---	-	---	---	---	--
3.3	---	-	---	---	---	---
0 (evap) <sup>3</sup>	+(+) <sup>4</sup>	---	---	---	---	---
1.3	---	---	+	+	+	-
2.3	---	---	+	+	+	-
3.3	---	---	-	-	+	-

28  
29

*Pyrococcus* GB-D

Treatment (hr.)	Pos. Ctrl <sup>1</sup>	25°C				
		0.5 N H <sub>2</sub> SO <sub>4</sub>	30% H <sub>2</sub> O <sub>2</sub>	20% H <sub>2</sub> O <sub>2</sub>	10% H <sub>2</sub> O <sub>2</sub>	DNA AWAY™
0 (evap) <sup>3</sup>	+(+) <sup>4</sup>	---	---	---	---	---
1.3	---	---	---	---	---	-
2.3	---	---	---	---	---	-
3.3	---	---	---	---	---	-

30

31 Aliquots (50  $\mu$ l) containing  $3 \times 10^4$  cells of *Euglena gracilis* were treated as indicated above.  
32 Aliquots (50  $\mu$ l) containing  $2 \times 10^8$  cells of *S. marinorubra* ( $H_2SO_4$  treatments);  $3 \times 10^7$  cells of  
33 *S. marinorubra* or *Pyrococcus sp.* ( $H_2O_2$  & DNA AWAY™ treatments) were treated as indicated  
34 above. The samples were extracted and taken through PCR amplification as described in  
35 Methods. PCR products were examined for the presence of DNA by agarose gel electrophoresis,  
36 followed by ethidium bromide staining. Visible DNA bands on the gels are indicated by a (+);  
37 no bands, by a (-). If not applicable or an experiment was not conducted, (---) was entered.  
38 <sup>1</sup>No treatment, positive control.  
39 <sup>2</sup>Reagent negative control.  
40 <sup>3</sup>Cell aliquot evaporated as in the  $H_2O_2$  and DNA AWAY™ treatments prior to DNA extraction.  
41 <sup>4</sup>Additional positive controls (+) in which cell aliquots were added to microfuge tubes in which  
42  $H_2O_2$  and DNAaway™ solutions that were evaporated indicated that remaining residues do not  
43 destroy DNA.  
44



45 **Table 4. Viability of *S. marinorubra* following exposure to hydrogen peroxide**  
 46 **(H<sub>2</sub>O<sub>2</sub>) and DNA AWAY™.**  
 47



Treatment Type	Exposure time (hr.)	Control Resuspended in 3.5% NaCl	Treatment Agent			
			H <sub>2</sub> O <sub>2</sub> (5%)	H <sub>2</sub> O <sub>2</sub> (10%)	H <sub>2</sub> O <sub>2</sub> (15%)	DNA AWAY™
I. Cells in Medium	1	---	-	-	-	---
	2	---	-	-	-	---
	3	---	-	-	-	---
	4	---	-	-	-	---
	5	---	-	-	-	---
	6	---	-	-	-	---
	7	---	-	-	-	---
	19	---	---	---	-	---
II. Pelleted Cells			H <sub>2</sub> O <sub>2</sub> (10%)	H <sub>2</sub> O <sub>2</sub> (20%)	H <sub>2</sub> O <sub>2</sub> (30%)	
	0.5	+	---	---	-	-
	1	+	-	-	-	-
	2	+	-	-	-	-
	3	+	-	-	-	-
	4	+	-	-	-	-
	5	+	-	-	-	-
	6	+	-	-	-	-
	7	+	-	-	-	-
	19	+	---	---	-	-
	22	+	---	---	-	-
	24	+	-	-	-	-
III. Cells added to Residue	1	+	---	---	+	+
	18	+	---	---	+	+
	41	+	---	---	+	+

48 Aliquots (50 µl) containing 4 x 10<sup>7</sup> cells of *S. marinorubra* were introduced into sterile  
 49 microfuge tubes and treated as indicated above (see also Methods). After treatment, 2µl aliquots  
 50 (1.6 x 10<sup>6</sup> cells) were spread onto the surface of Marine Agar 2216 plates for growth.  
 51 Appearance of one or more colonies after 7 days incubation at room temperature scored as (+),  
 52 no colonies scored as (-). If not applicable or an experiment was not conducted, (---) was  
 53 entered.  
 54

55 **Treatment I.** Cells in Marine Broth 2216 cultures exposed to H<sub>2</sub>O<sub>2</sub> at the indicated final  
 56 concentration.

57 **Treatment II.** Cells from above broth cultures centrifuged to remove medium and exposed to  
 58 H<sub>2</sub>O<sub>2</sub> at the indicated final concentrations. Control cultures were resuspended in 3.5% NaCl.

59 ***Treatment III.*** Cells in Marine Broth 2216 cultures added to sterile microfuge tubes in which  
60 H<sub>2</sub>O<sub>2</sub> and DNA AWAY™ were evaporated to determine if toxic residues were left behind after  
61 evaporation.

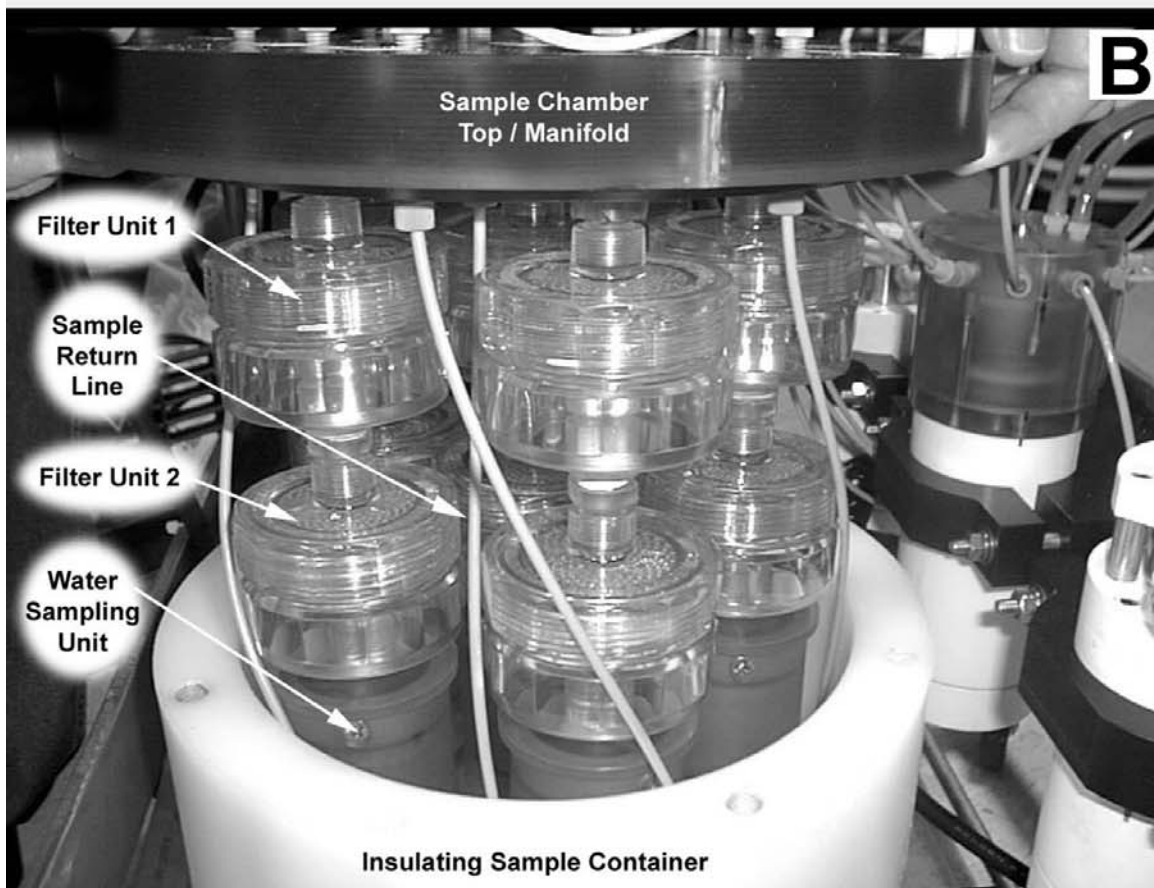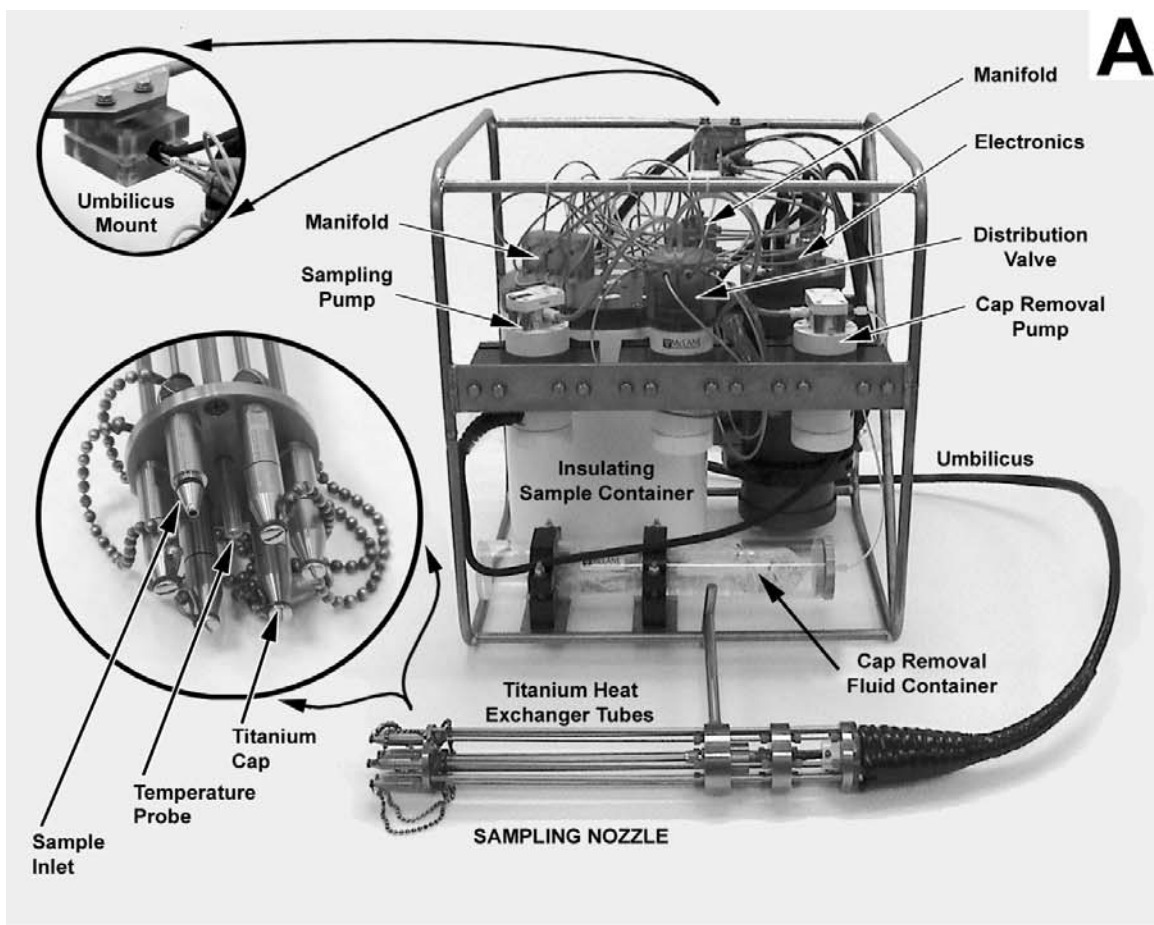






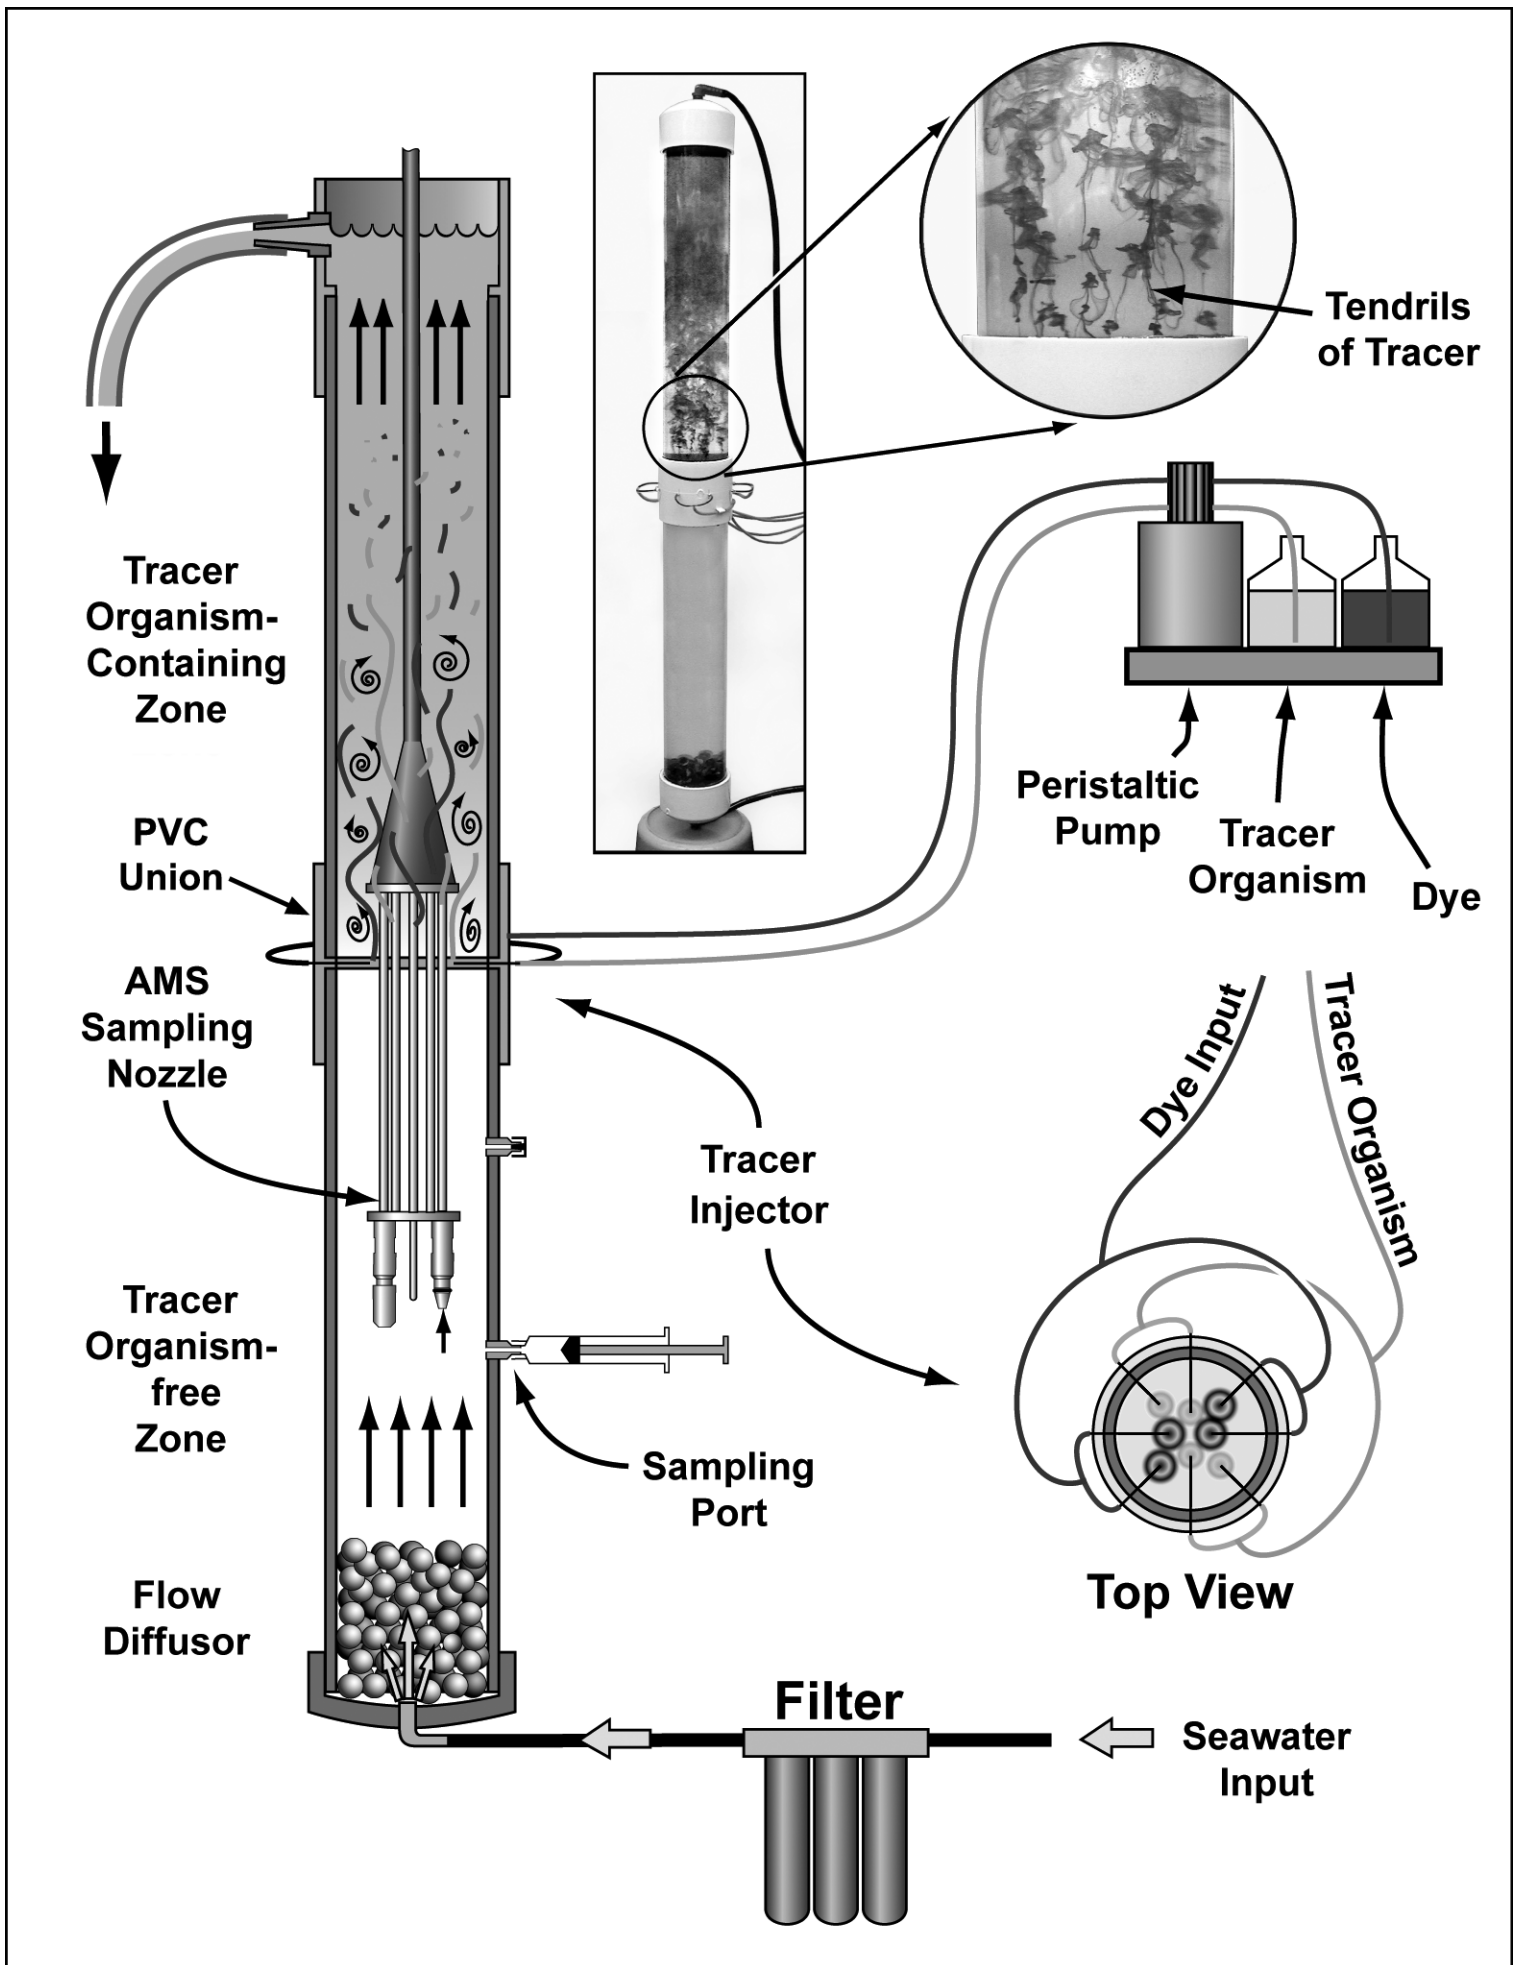


Figure 3

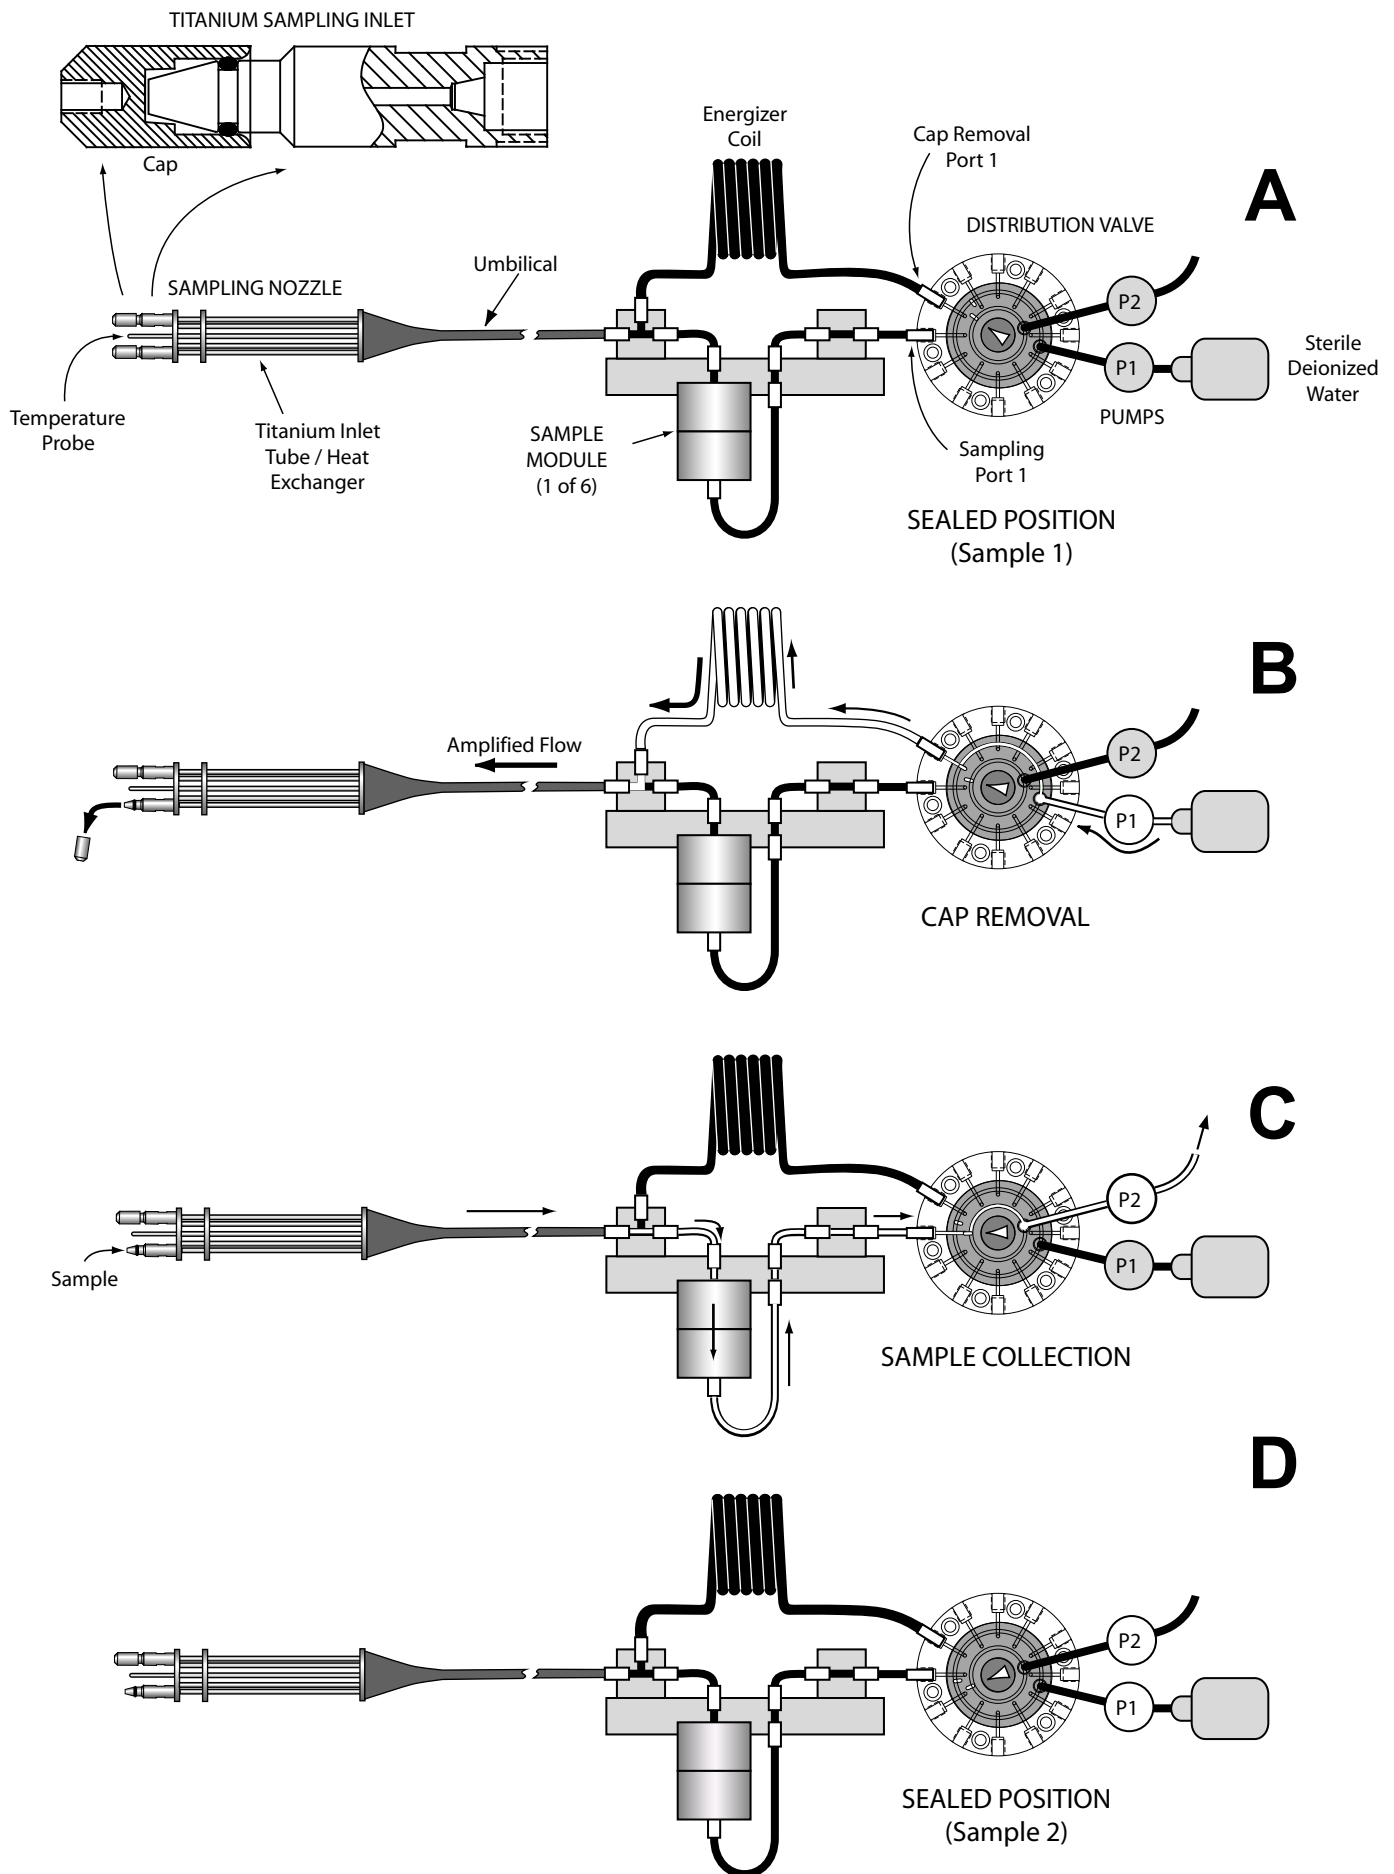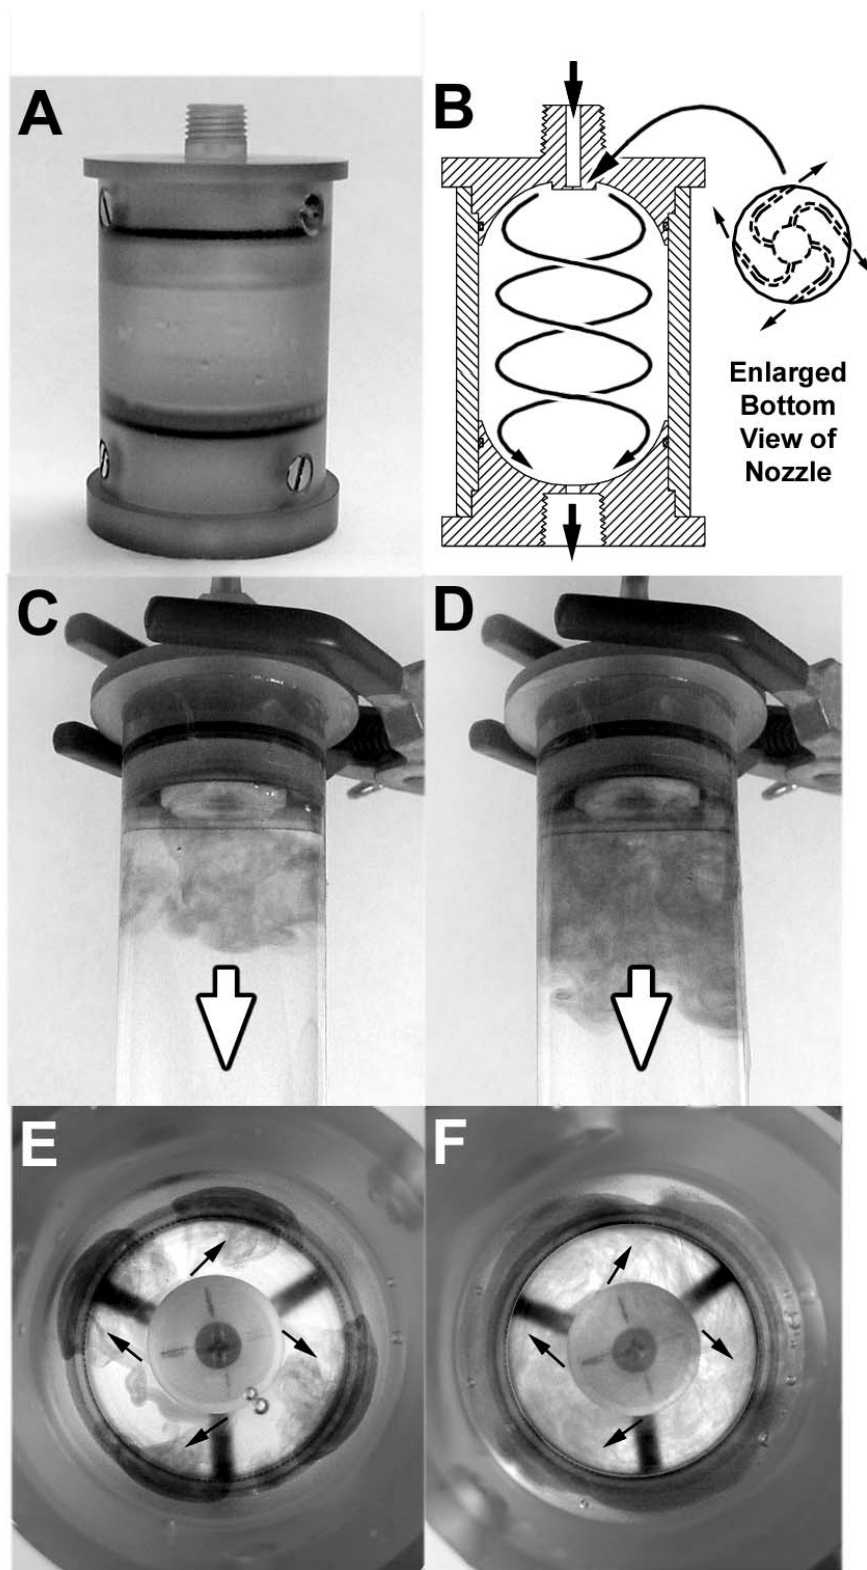



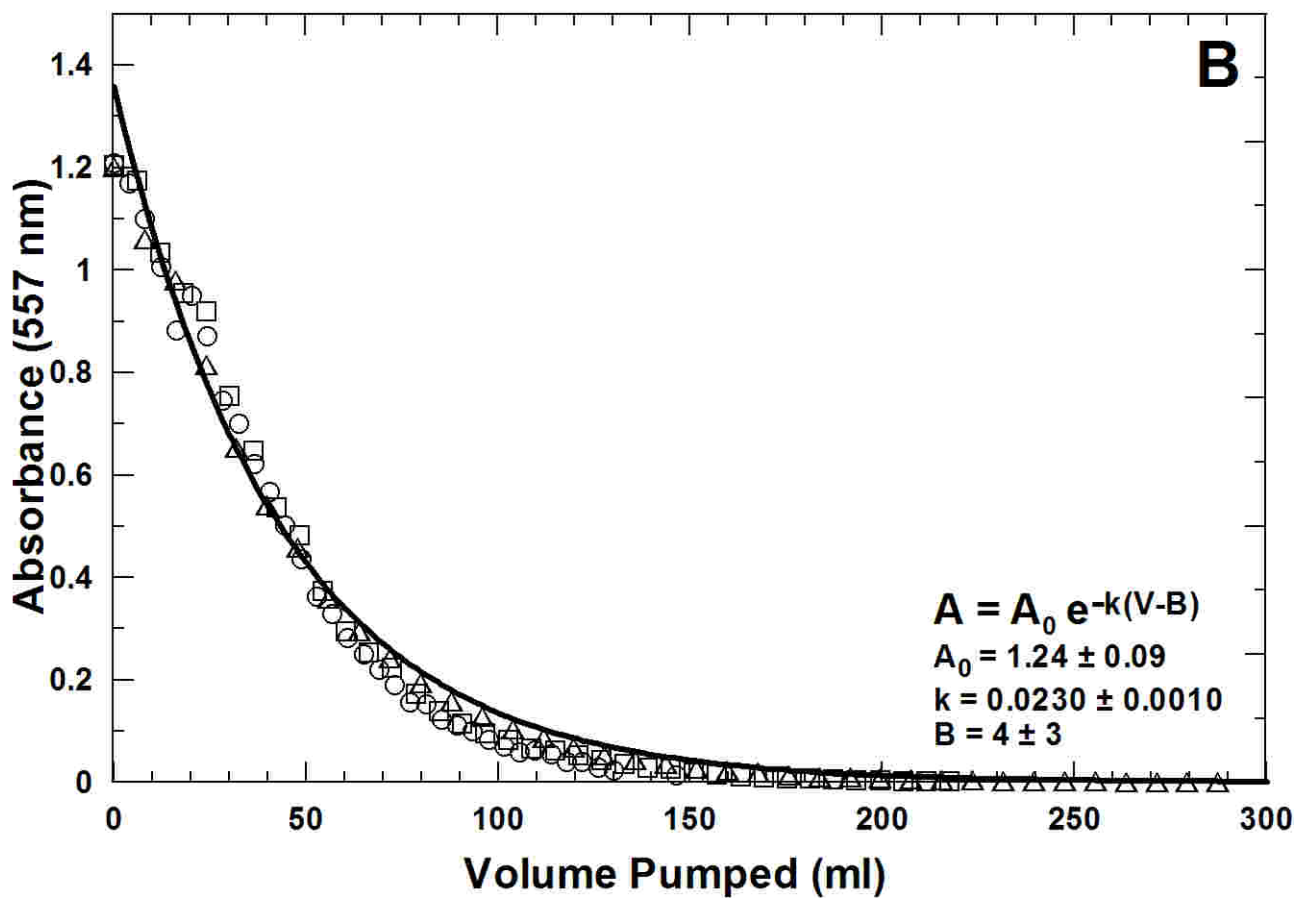


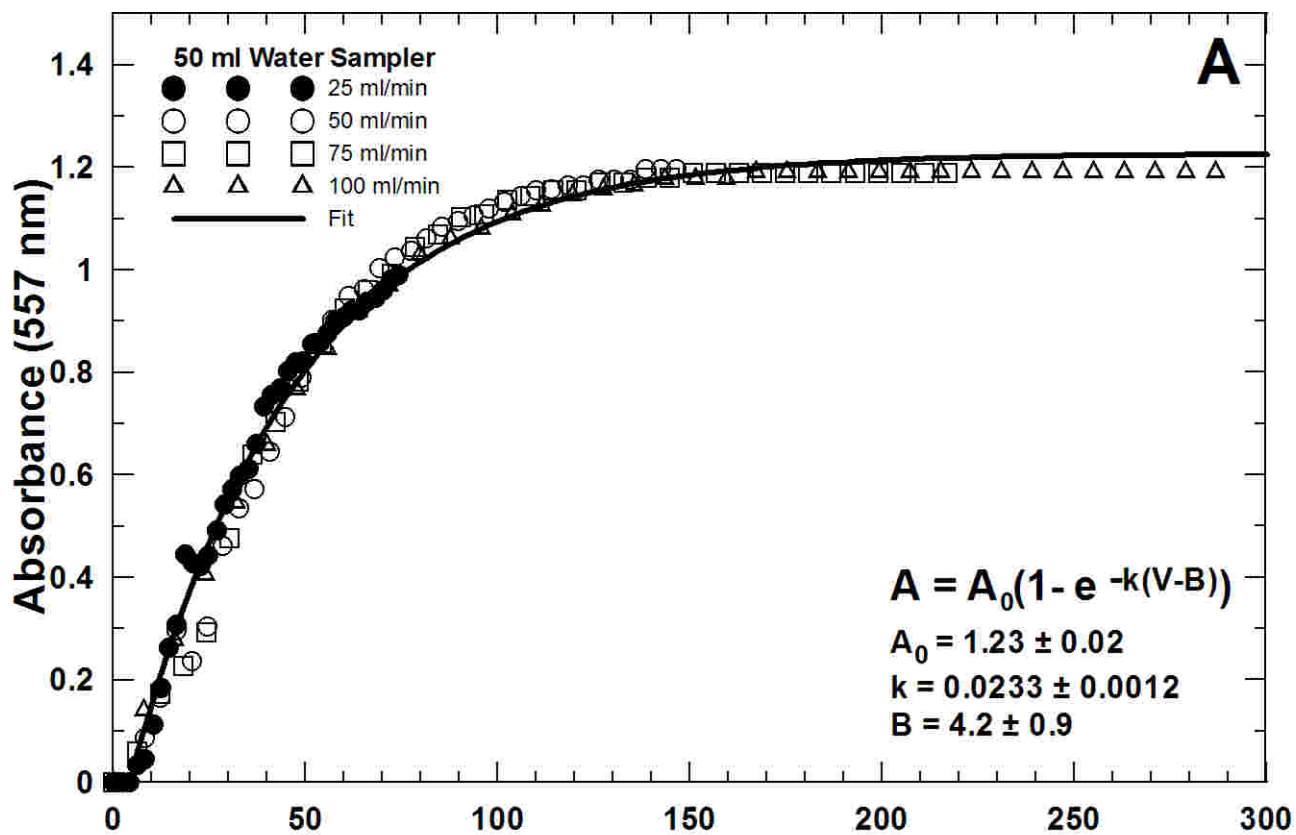

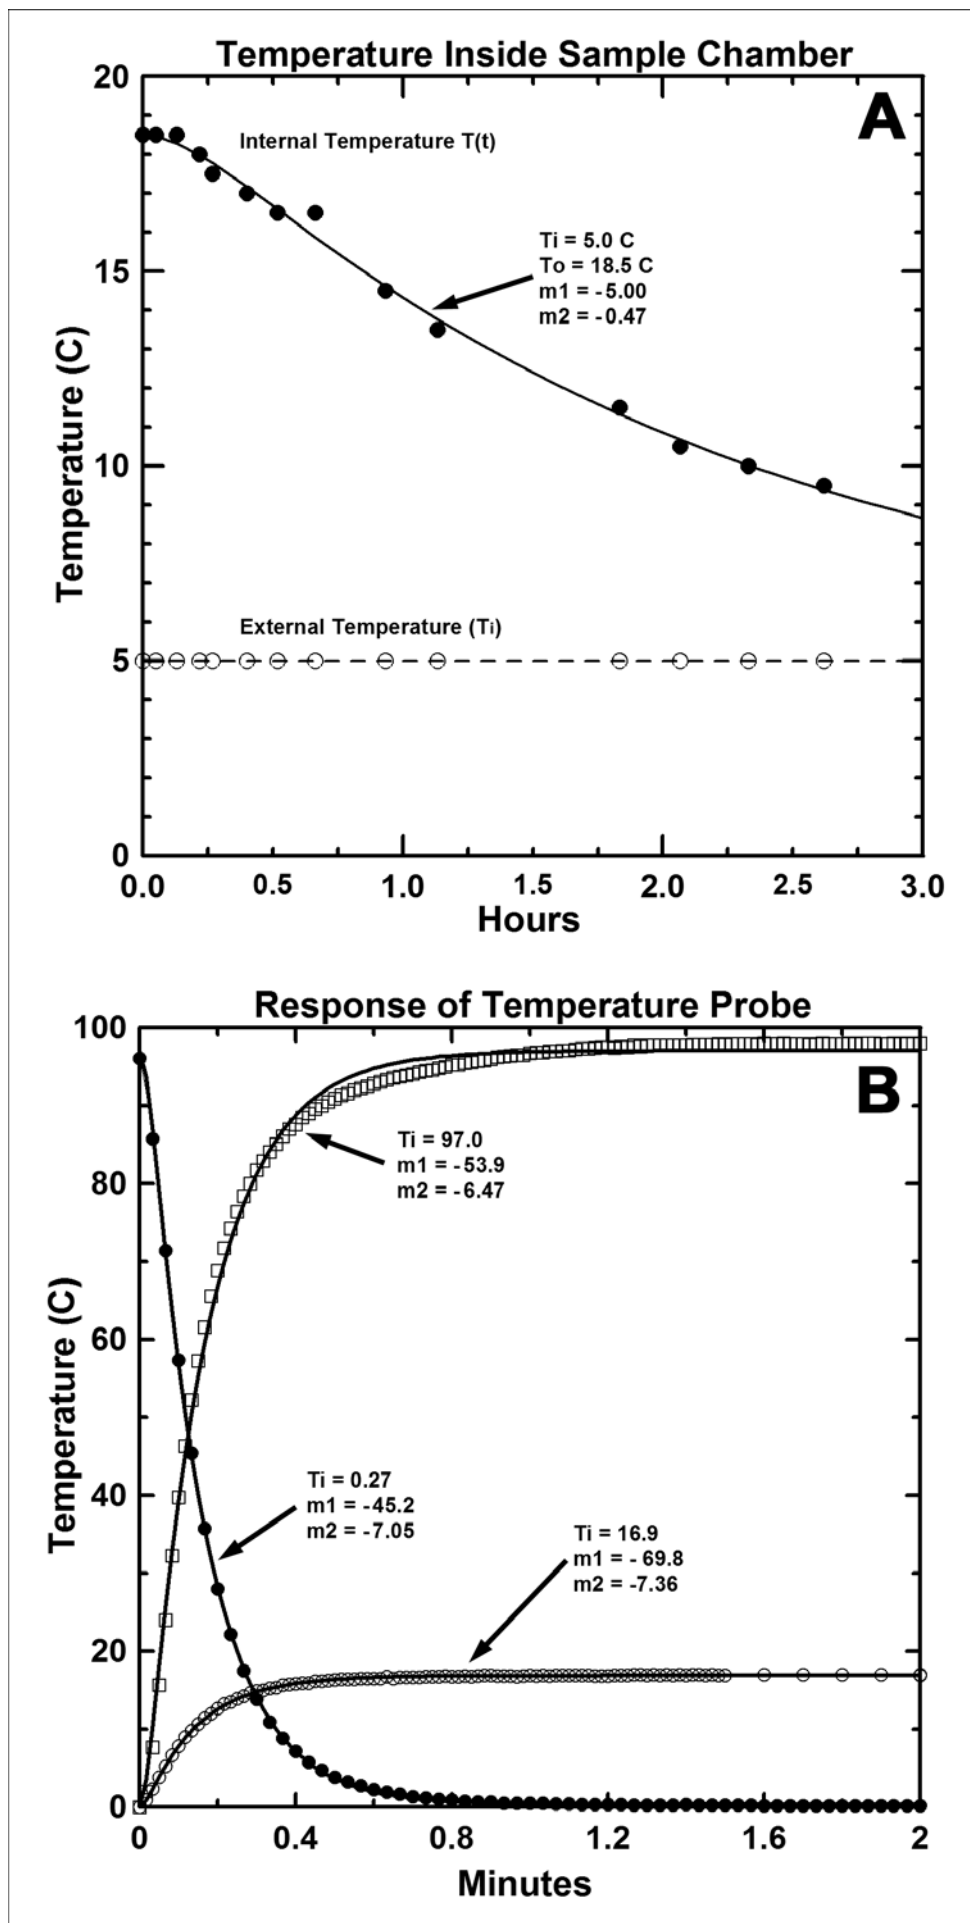




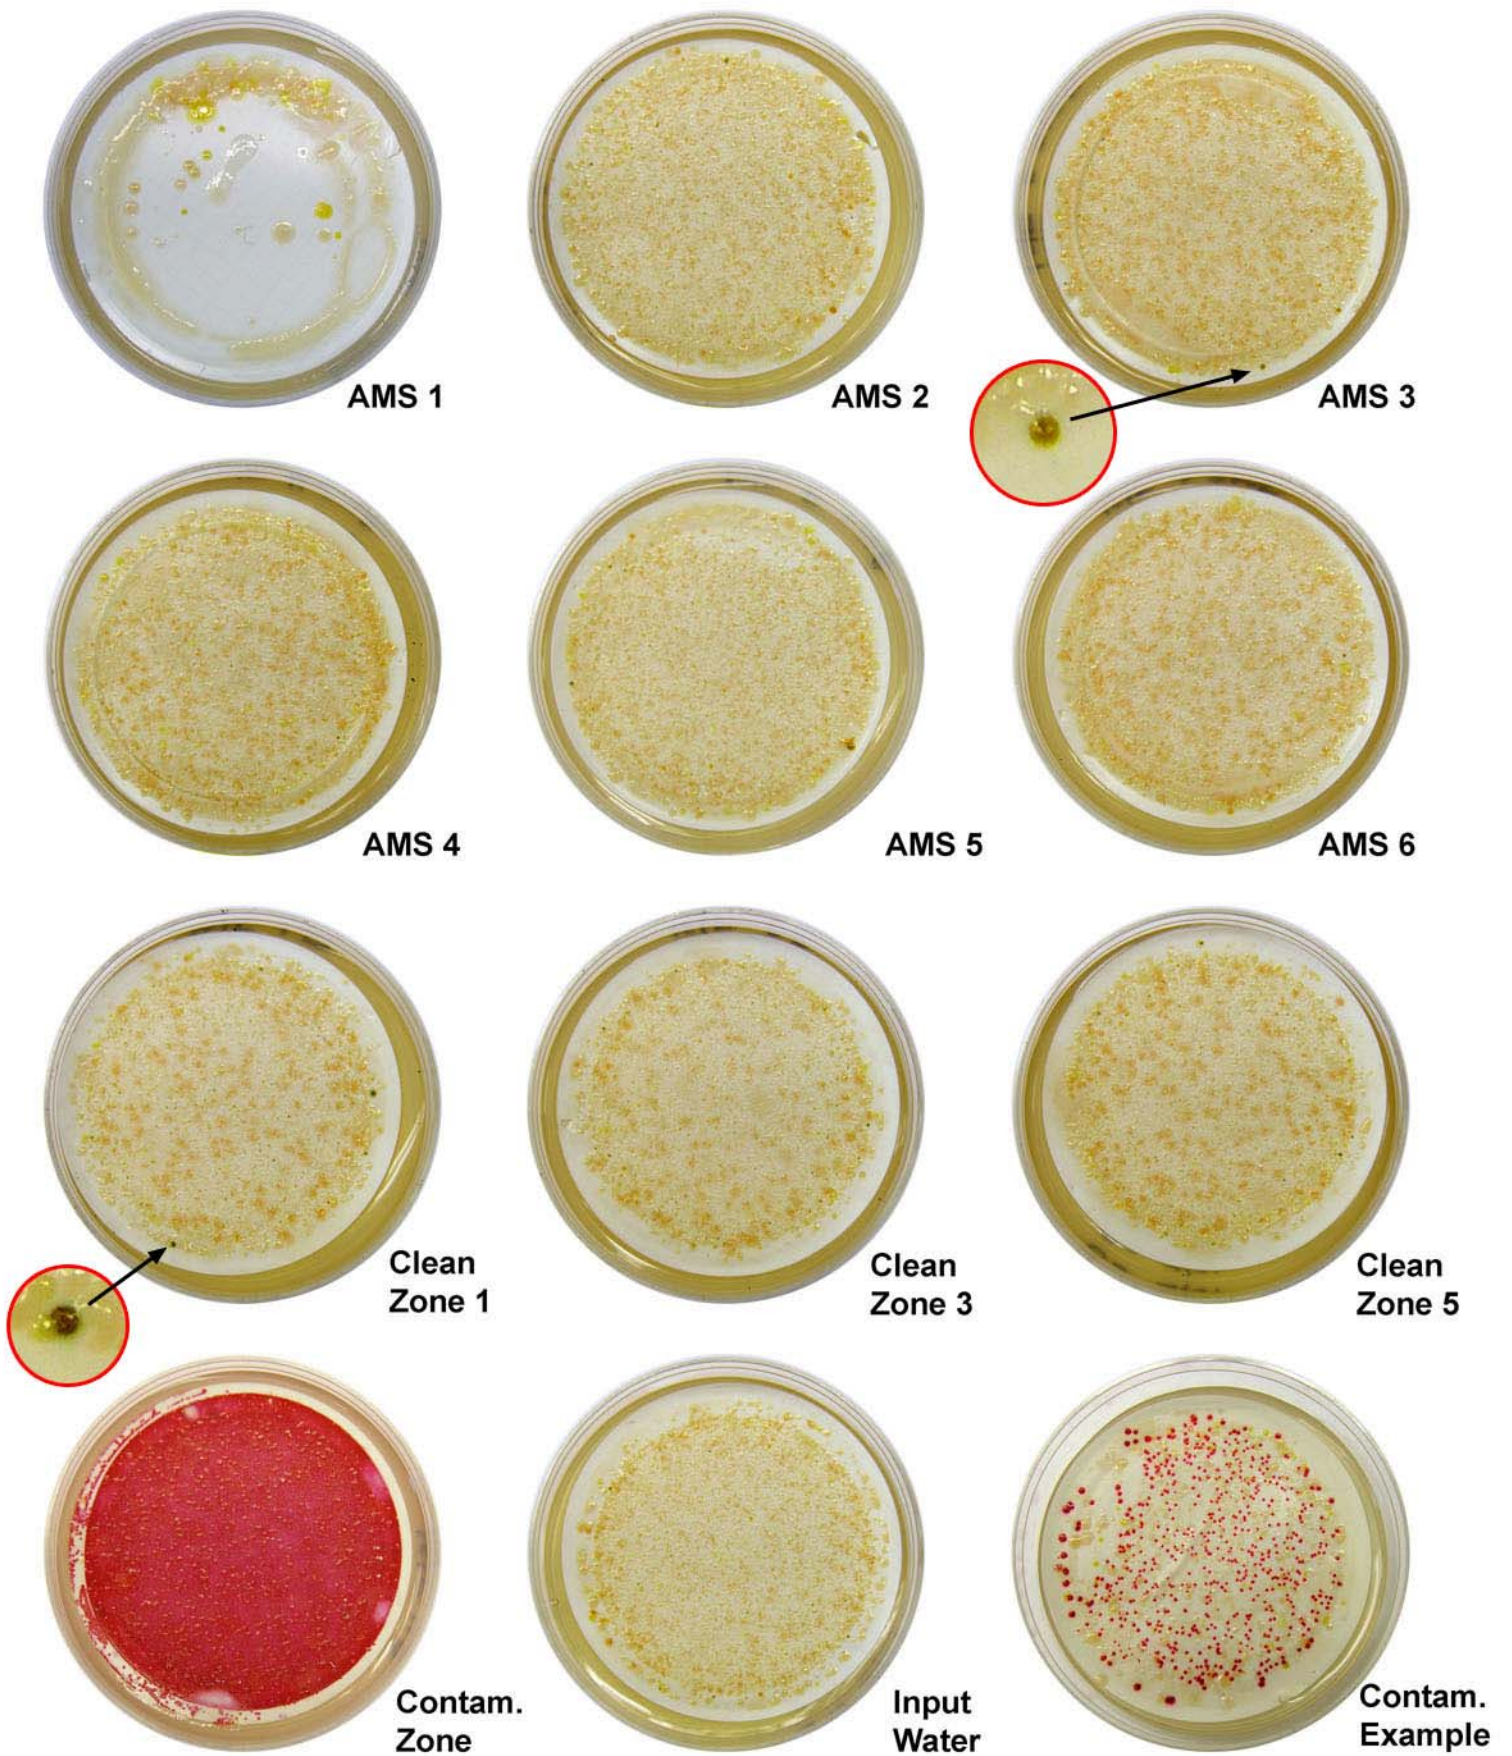

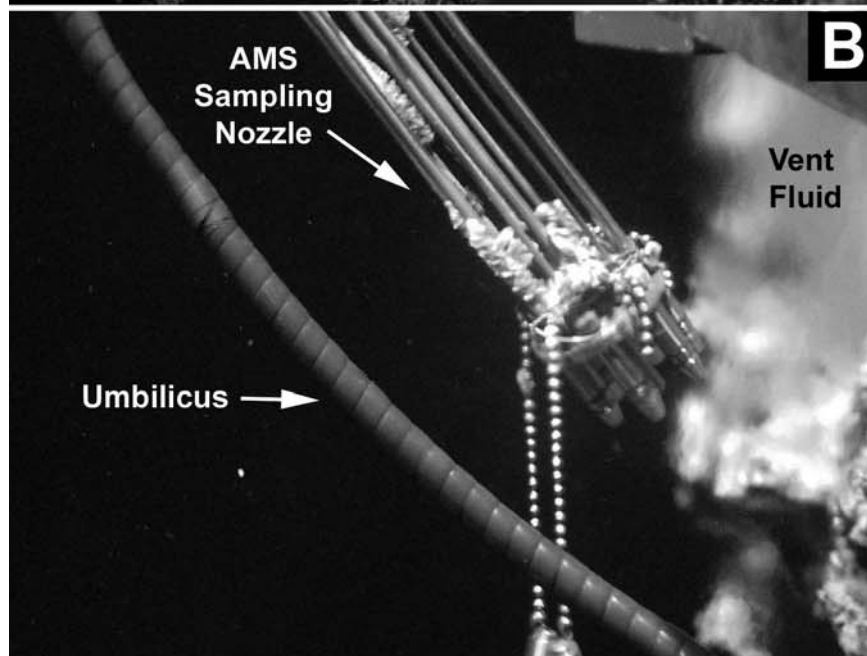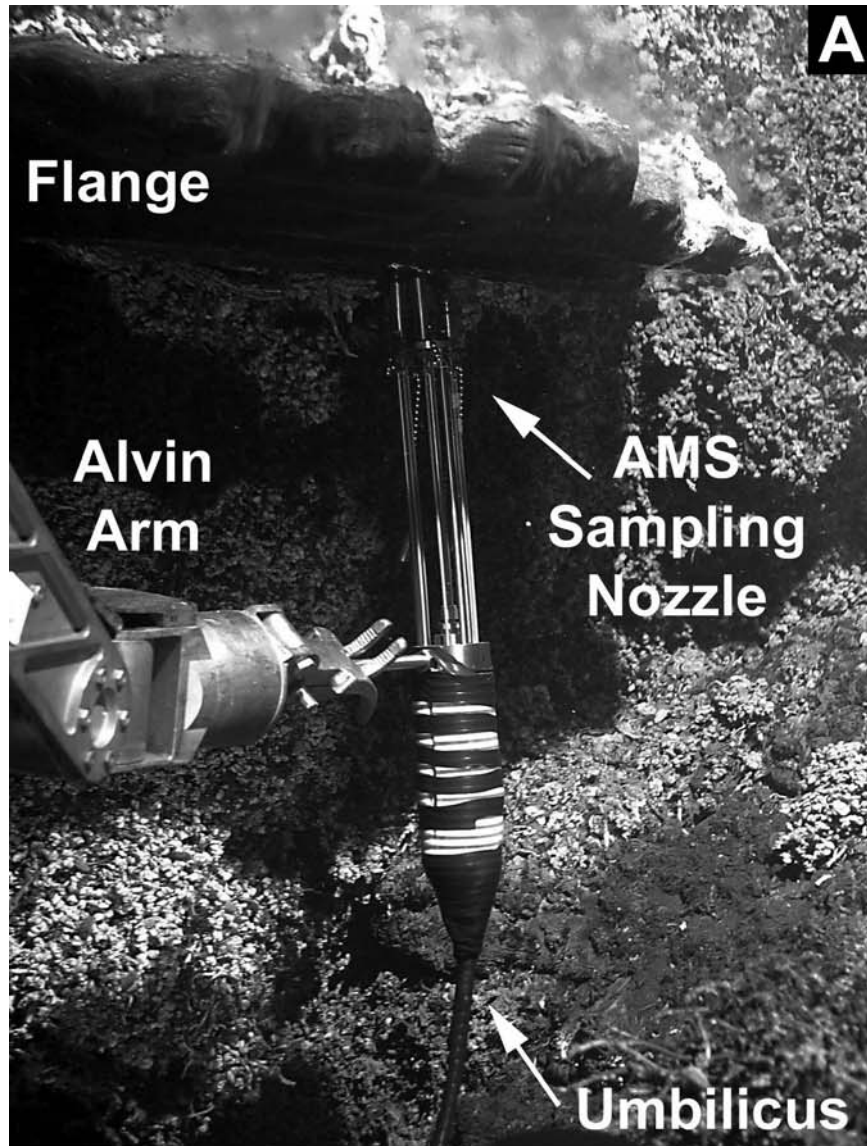

Gel 1

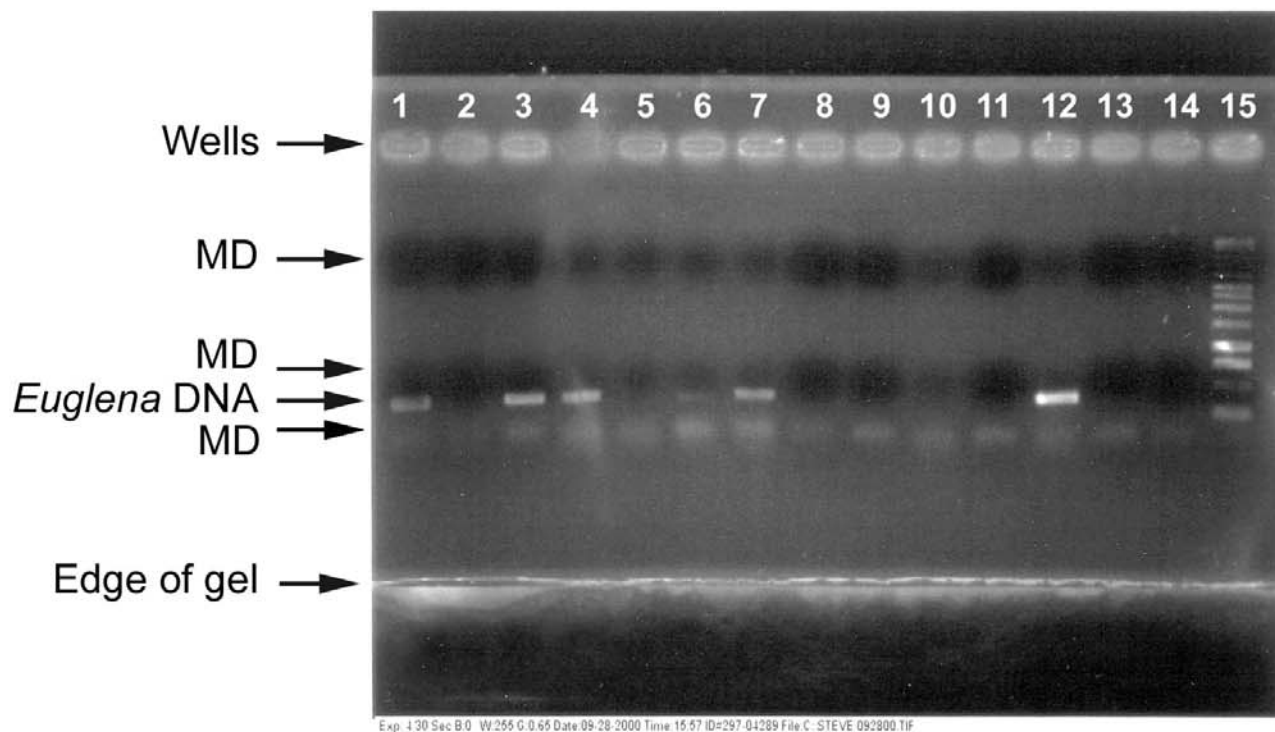

Gel 2

